

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0063025\
 Data File : P0111907.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jun 2025 17:38
 Operator : YP/AJ
 Sample : Q2451-01 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 Y2310-0409-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/01/2025
 Supervised By :mohammad ahmed 07/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 01:36:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.674	3.671	7414616	5681217	1.287	1.011m
2) SA Decachlor...	8.702	8.654	4402657	1942505	0.839m	1.093m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO063025\
Data File : PO111907.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jun 2025 17:38
Operator : YP/AJ
Sample : Q2451-01 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
Y2310-0409-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 01:36:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

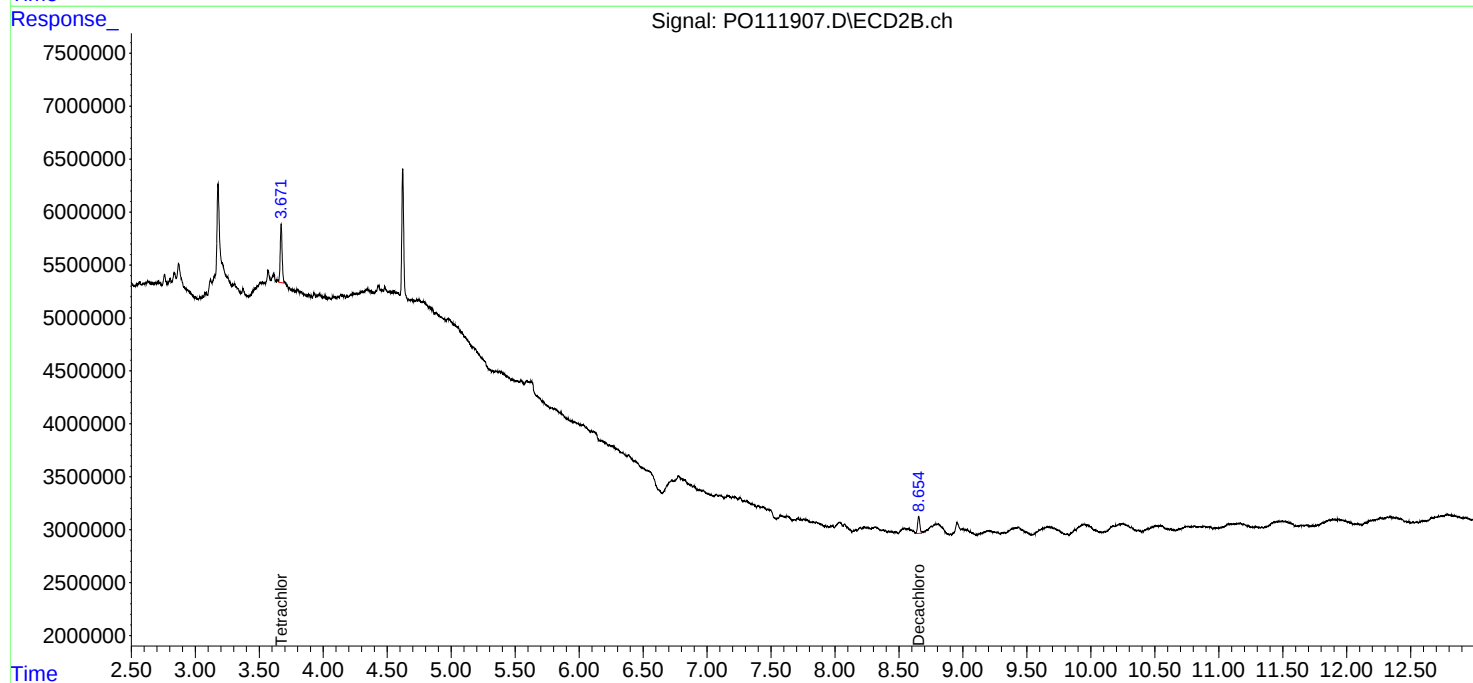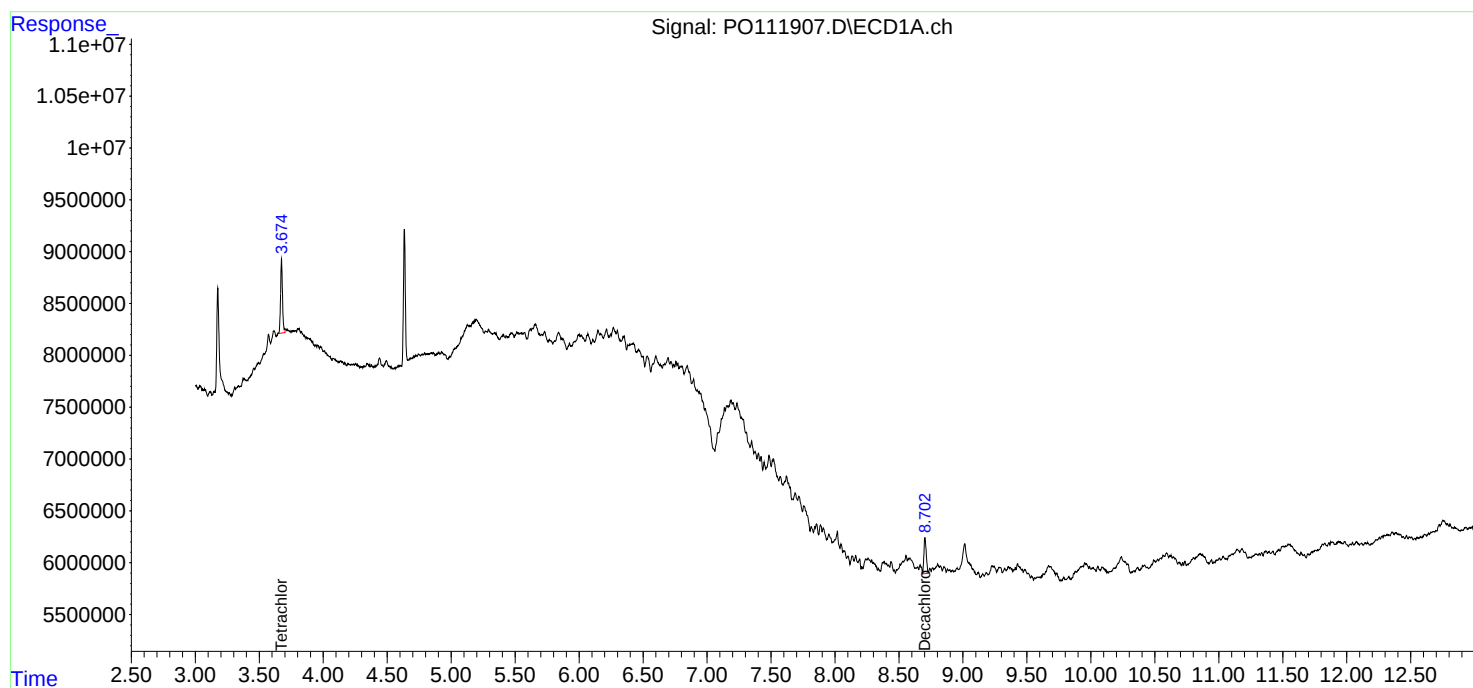

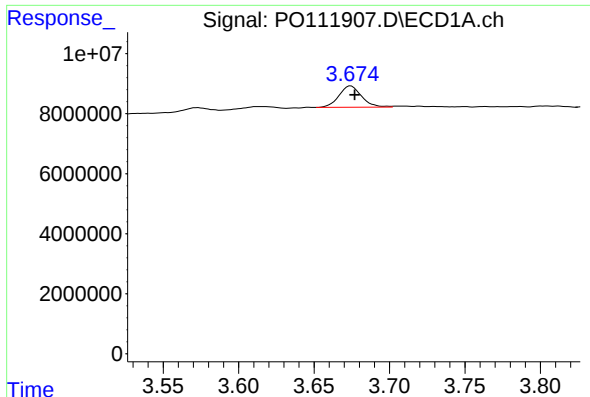


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 7414616
Conc: 1.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
Y2310-0409-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/01/2025
Supervised By :mohammad ahmed 07/01/2025

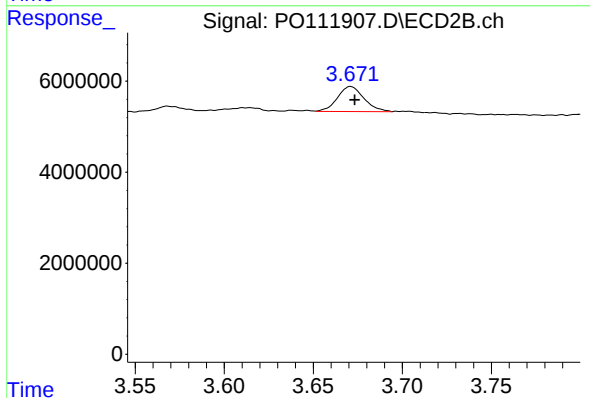


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.003 min
Response: 5681217
Conc: 1.01 ng/ml m

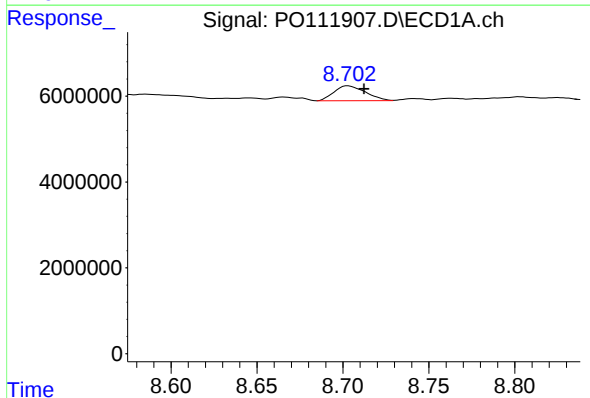

#2 Decachlorobiphenyl

R.T.: 8.702 min
Delta R.T.: -0.010 min
Response: 4402657
Conc: 0.84 ng/ml m

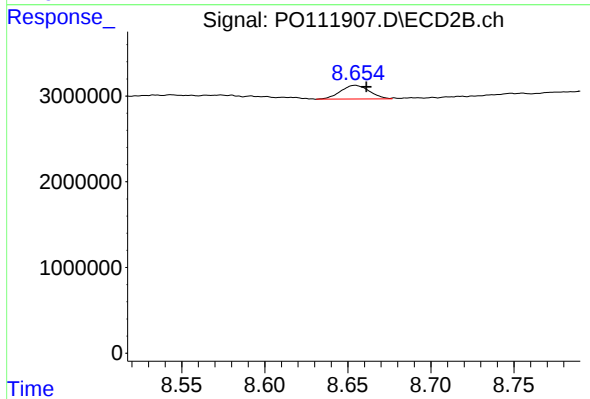

#2 Decachlorobiphenyl

R.T.: 8.654 min
Delta R.T.: -0.007 min
Response: 1942505
Conc: 1.09 ng/ml m