

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
 Data File : P0057632.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 12:09
 Operator : SM/SJ
 Sample : K3507-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NB-07-062619-A

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:39:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 13:40:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.226	3.551	972333	779256	24.753	22.161
2) SA Decachlor...	9.765	8.468	864881	553381	15.380m	14.794

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070119\
Data File : PO057632.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 12:09
Operator : SM/SJ
Sample : K3507-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NB-07-062619-A


Manual Integrations
APPROVED

Ankita
7/2/2019 1:39:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 13:40:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

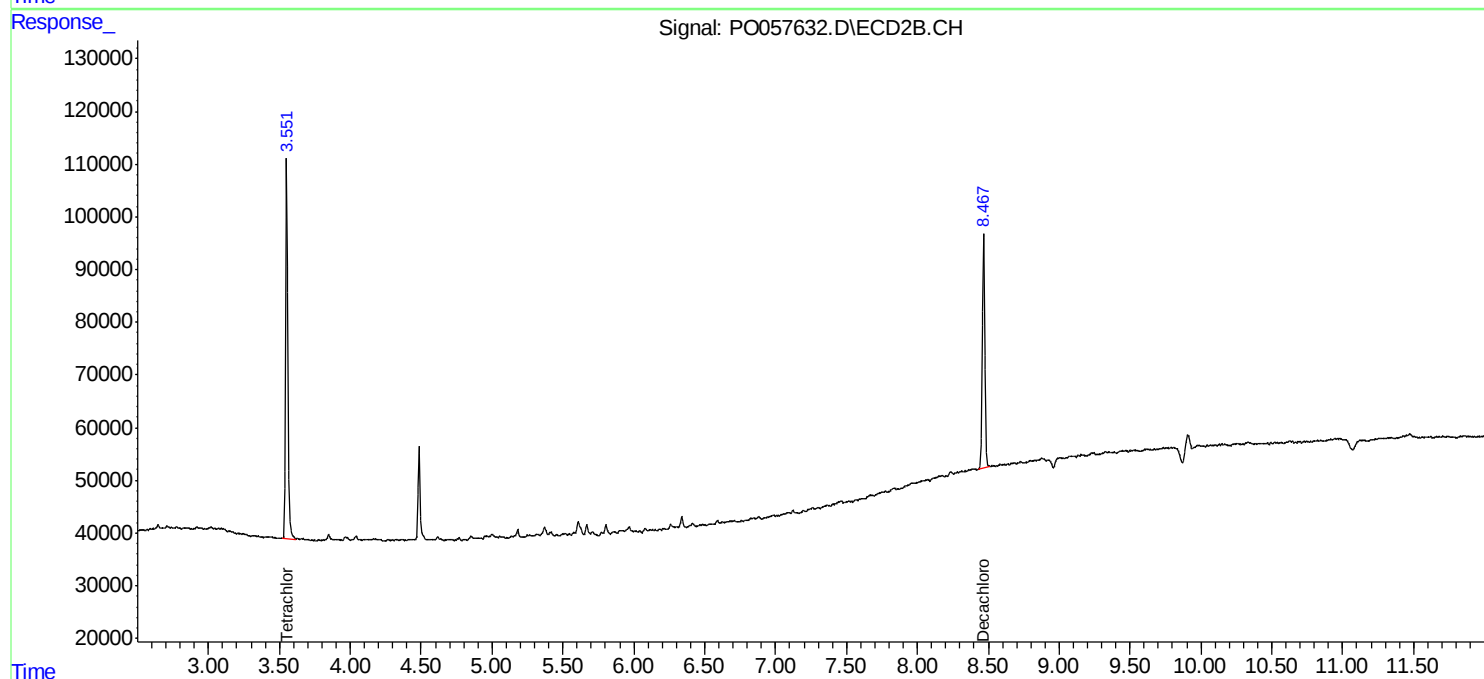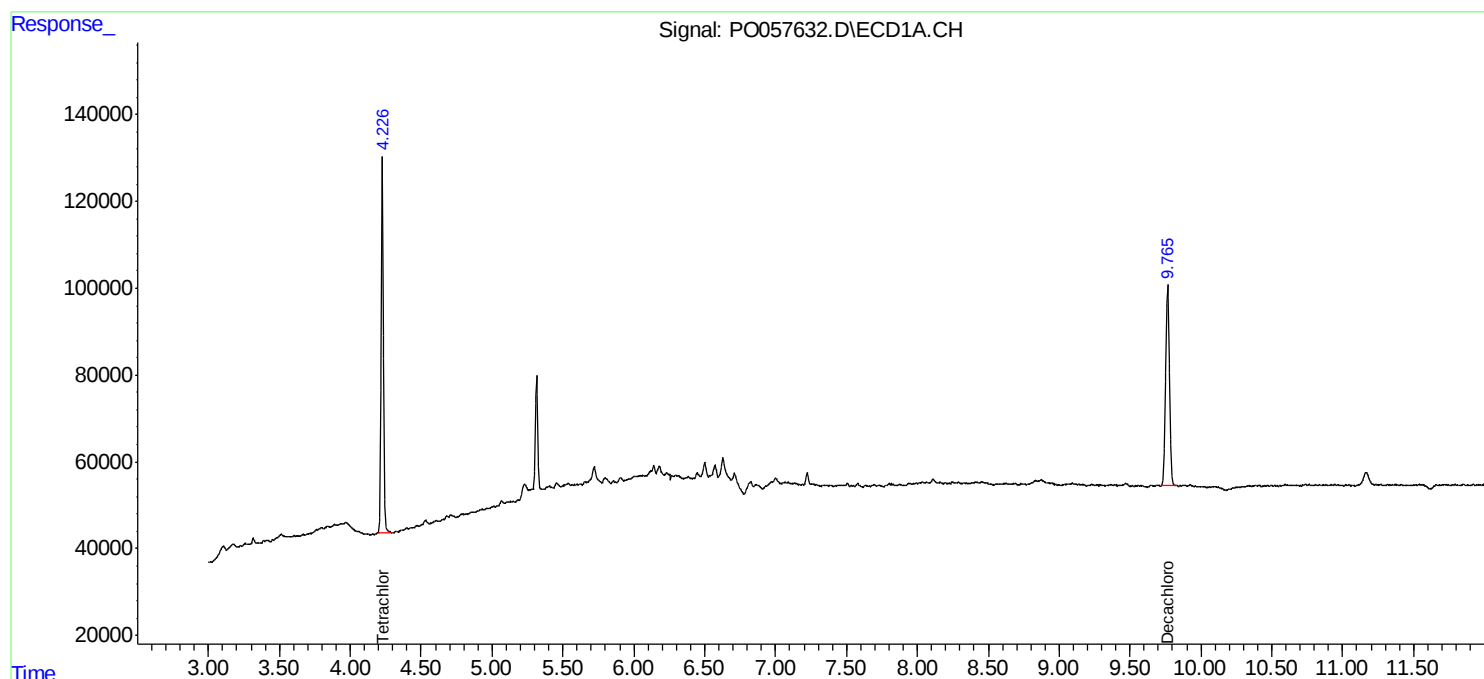

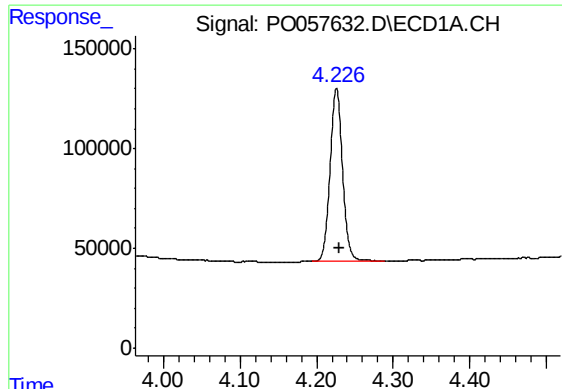


#1 Tetrachloro-m-xylene

R.T.: 4.226 min
Delta R.T.: -0.004 min
Response: 972333
Conc: 24.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
NB-07-062619-A


Manual Integrations
APPROVED

Ankita
7/2/2019 1:39:42 PM

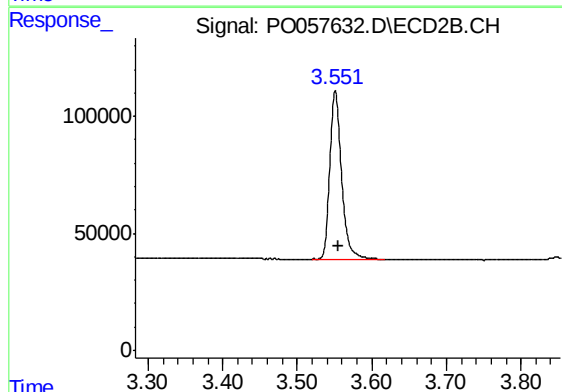


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.004 min
Response: 779256
Conc: 22.16 ng/ml

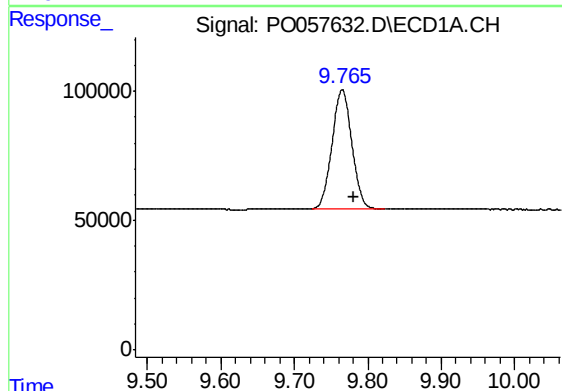

#2 Decachlorobiphenyl

R.T.: 9.765 min
Delta R.T.: -0.016 min
Response: 864881
Conc: 15.38 ng/ml m

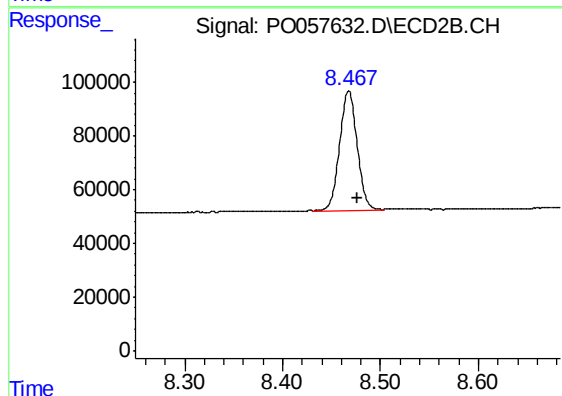

#2 Decachlorobiphenyl

R.T.: 8.468 min
Delta R.T.: -0.009 min
Response: 553381
Conc: 14.79 ng/ml