

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
 Data File : P0057634.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 12:50
 Operator : SM/SJ
 Sample : PB121034BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB121034BL

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:39:46 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 13:41:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.226	3.551	812504	660431	20.684	18.782
2)	SA Decachlor...	9.767	8.467	882921	563619	15.701m	15.067

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
Data File : P0057634.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 12:50
Operator : SM/SJ
Sample : PB121034BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB121034BL


Manual Integrations
APPROVED

Ankita
7/2/2019 1:39:46 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 13:41:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

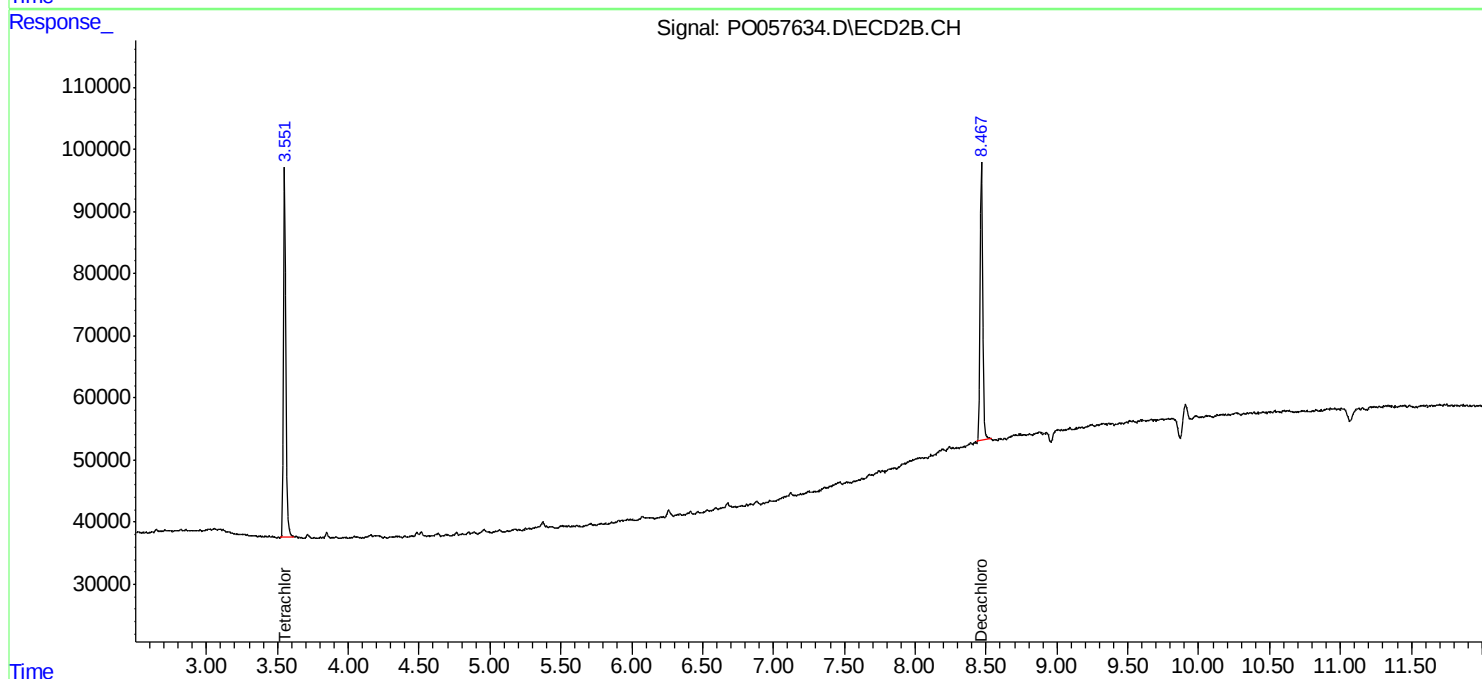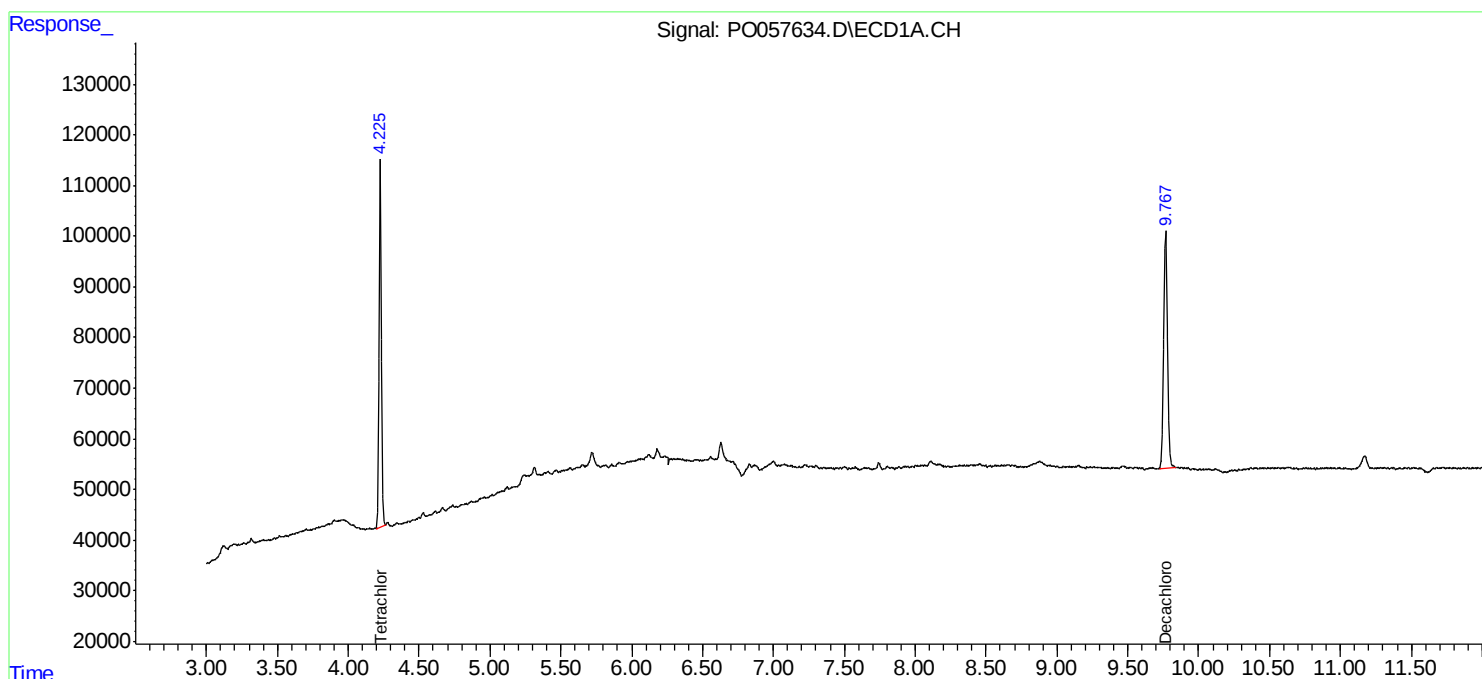

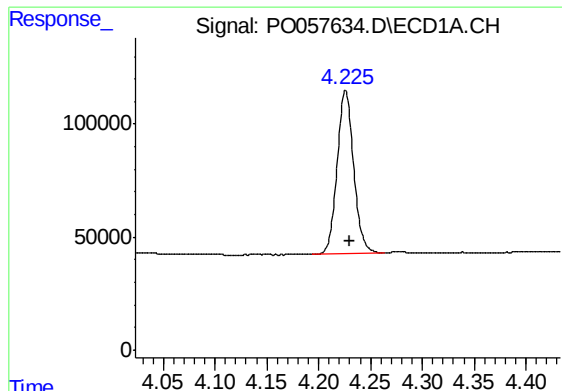


#1 Tetrachloro-m-xylene

R.T.: 4.226 min
Delta R.T.: -0.004 min
Response: 812504
Conc: 20.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB121034BL


Manual Integrations
APPROVED

Ankita
7/2/2019 1:39:46 PM

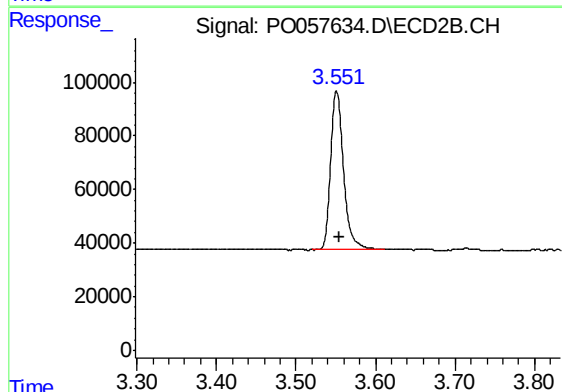


#1 Tetrachloro-m-xylene

R.T.: 3.551 min
Delta R.T.: -0.004 min
Response: 660431
Conc: 18.78 ng/ml

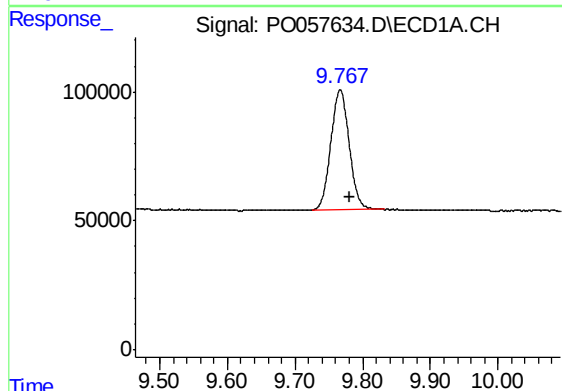

#2 Decachlorobiphenyl

R.T.: 9.767 min
Delta R.T.: -0.015 min
Response: 882921
Conc: 15.70 ng/ml m

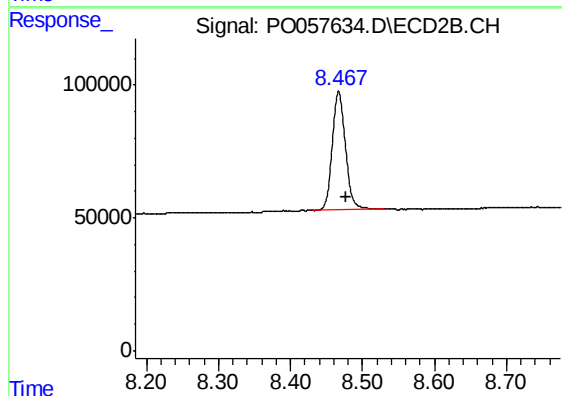

#2 Decachlorobiphenyl

R.T.: 8.467 min
Delta R.T.: -0.010 min
Response: 563619
Conc: 15.07 ng/ml