

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
Data File : P0057658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 20:58
Operator : SM/SJ
Sample : K3564-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 08:26:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.217	3.549	662908	567673	16.876	16.144
2)	SA Decachlor...	9.756	8.465	673709	451848	11.981	12.079

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
Data File : P0057658.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 20:58
Operator : SM/SJ
Sample : K3564-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 08:26:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

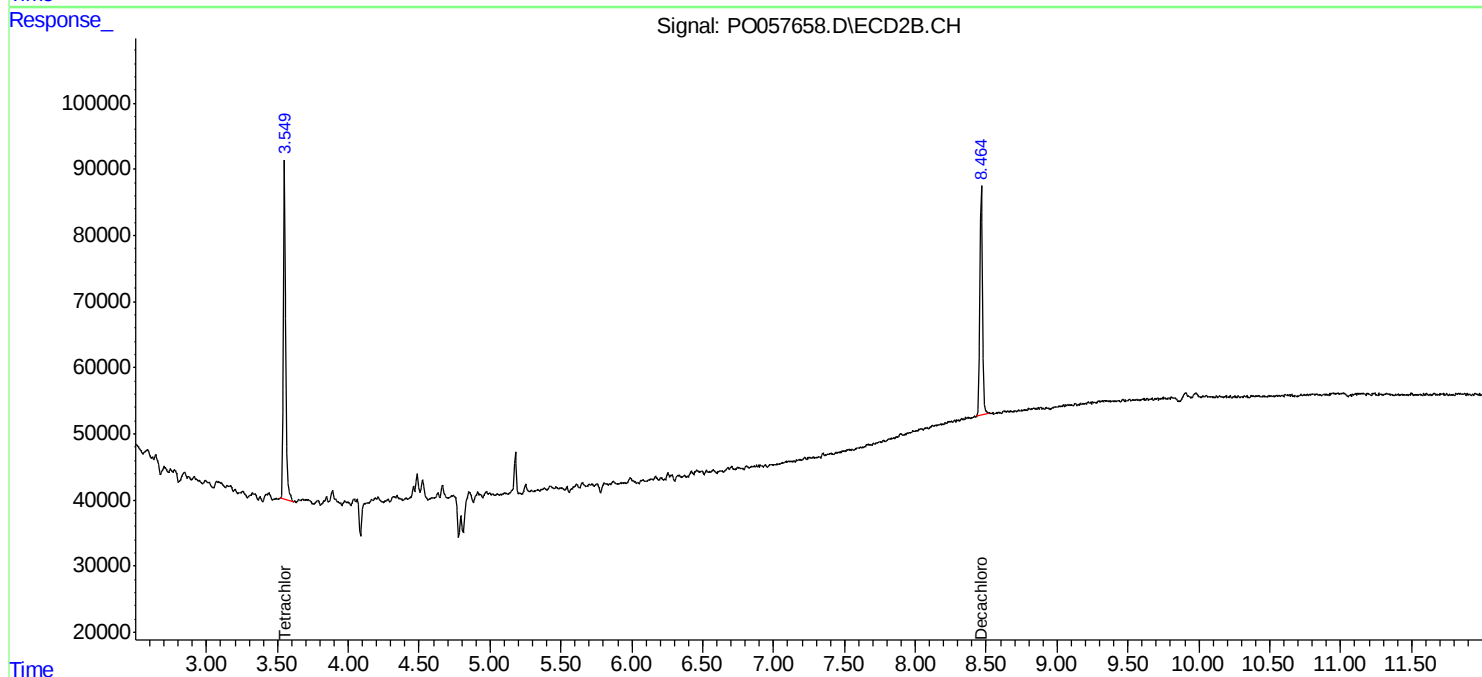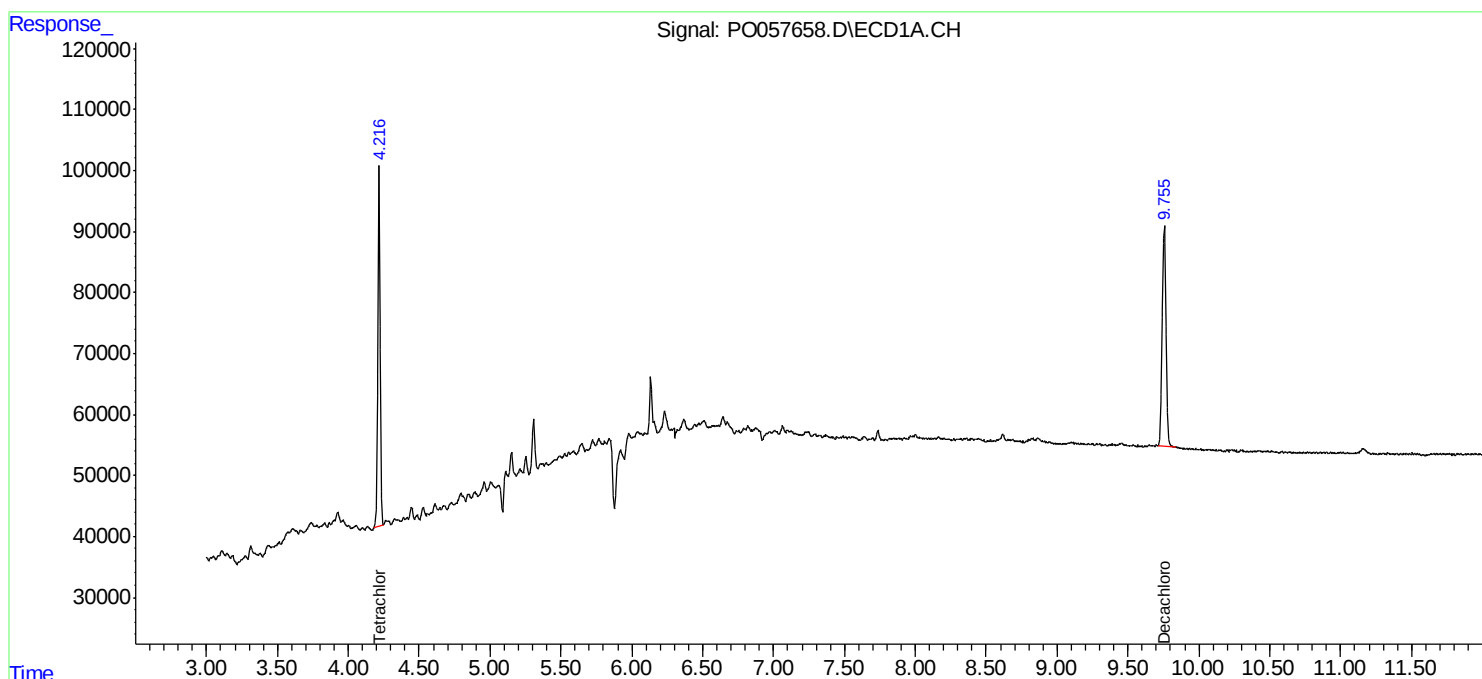


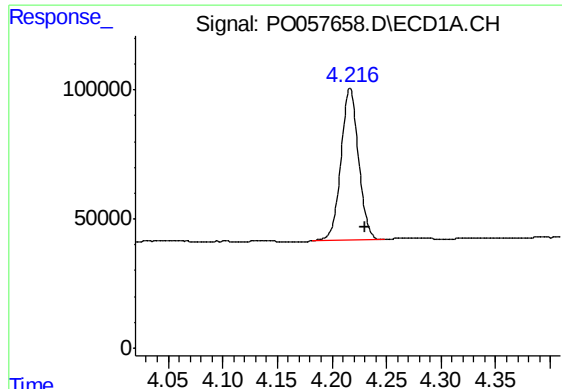

#1 Tetrachloro-m-xylene


R.T.: 4.217 min
Delta R.T.: -0.013 min
Response: 662908
Conc: 16.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-1

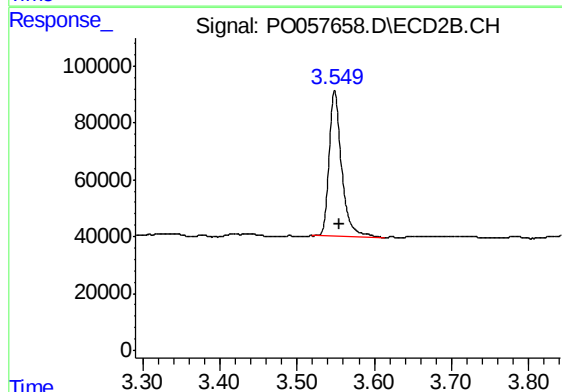


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.006 min
Response: 567673
Conc: 16.14 ng/ml

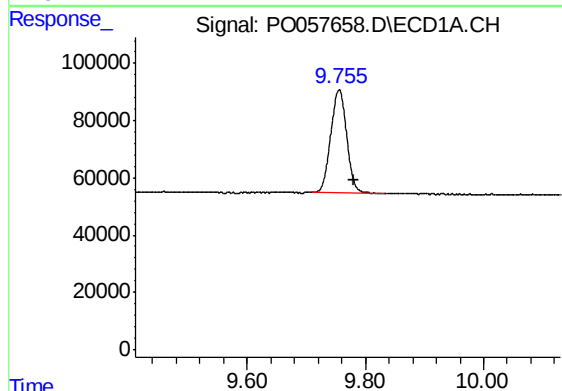

#2 Decachlorobiphenyl

R.T.: 9.756 min
Delta R.T.: -0.026 min
Response: 673709
Conc: 11.98 ng/ml

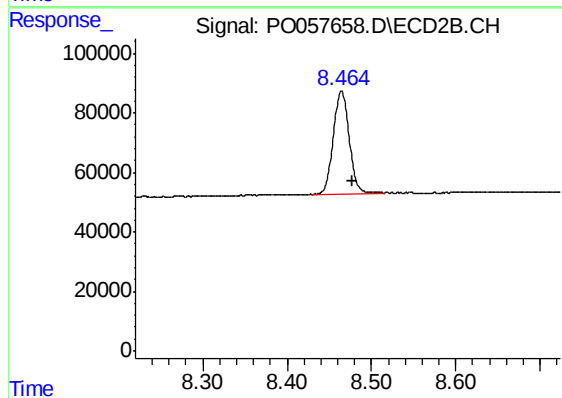

#2 Decachlorobiphenyl

R.T.: 8.465 min
Delta R.T.: -0.012 min
Response: 451848
Conc: 12.08 ng/ml