

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070119\
 Data File : P0057661.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2019 21:49
 Operator : SM/SJ
 Sample : K3585-12
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RM-WATER-COMP

Manual Integrations
 APPROVED

Ankita
 7/2/2019 1:40:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 08:32:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.217	3.549	873984	1092308	22.249m	31.064m#
2)	SA Decachlor...	9.756	8.463	871986	591123	15.507	15.803

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070119\
Data File : PO057661.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2019 21:49
Operator : SM/SJ
Sample : K3585-12
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
RM-WATER-COMP


Manual Integrations
APPROVED

Ankita
7/2/2019 1:40:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 08:32:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

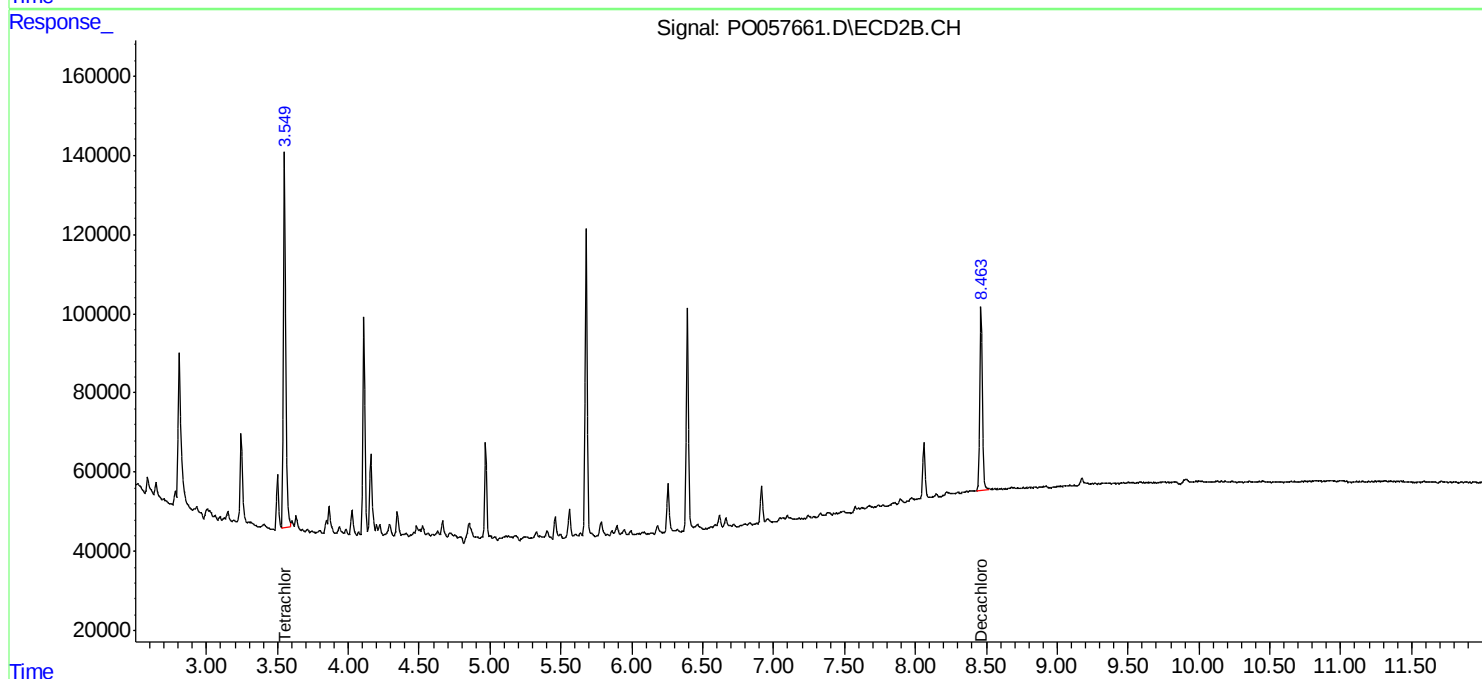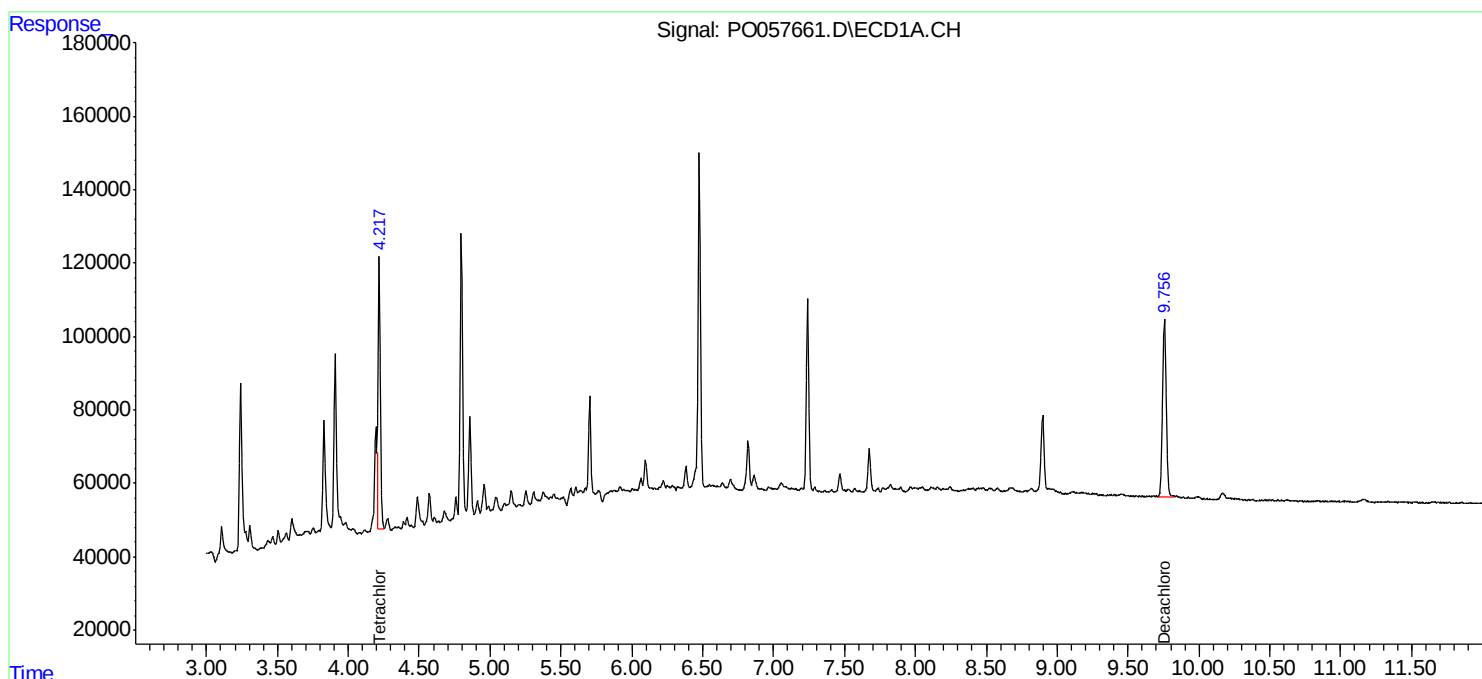

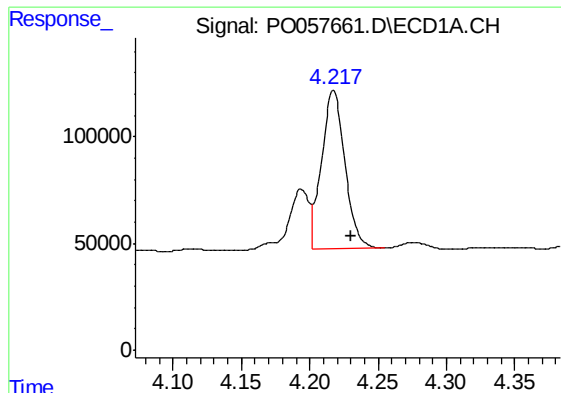


#1 Tetrachloro-m-xylene

R.T.: 4.217 min
Delta R.T.: -0.013 min
Response: 873984
Conc: 22.25 ng/ml m

Instrument :
ECD_O
ClientSampleId :
RM-WATER-COMP


Manual Integrations
APPROVED

Ankita
7/2/2019 1:40:37 PM

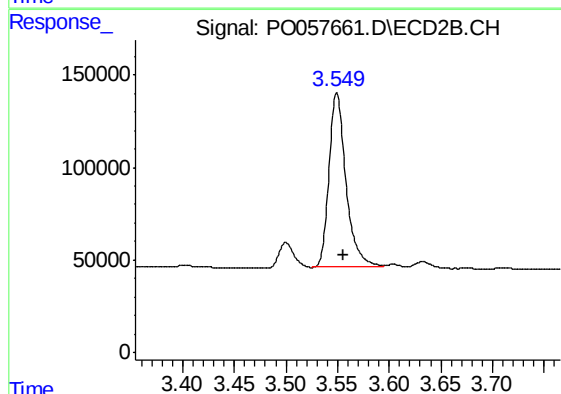


#1 Tetrachloro-m-xylene

R.T.: 3.549 min
Delta R.T.: -0.006 min
Response: 1092308
Conc: 31.06 ng/ml m

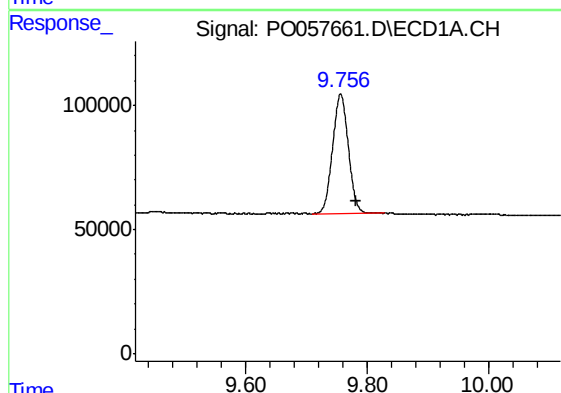

#2 Decachlorobiphenyl

R.T.: 9.756 min
Delta R.T.: -0.025 min
Response: 871986
Conc: 15.51 ng/ml

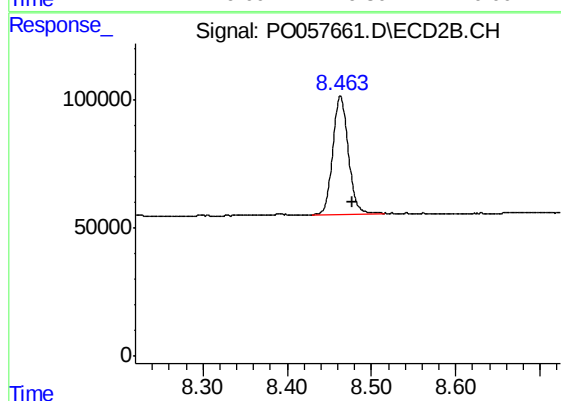

#2 Decachlorobiphenyl

R.T.: 8.463 min
Delta R.T.: -0.014 min
Response: 591123
Conc: 15.80 ng/ml