

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
 Data File : P0069346.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2020 12:46
 Operator : DD\AJ
 Sample : L3157-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CB-D35

Manual Integrations
 APPROVED

Ankita
 7/2/2020 10:44:47 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 13:50:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.401	3.566	804741	915549	27.203	23.787
2) SA Decachlor...	10.066	8.776	947483	993743	19.949	18.255
Target Compounds						
31) L7 AR-1260-1	7.373	6.366	194466	290020	101.898m	123.943
32) L7 AR-1260-2	7.641	6.566	260041	333805	111.104	117.268
33) L7 AR-1260-3	8.001	6.713	272145	255970	153.187	95.171 #
34) L7 AR-1260-4	8.226	7.193	339328	284718	162.713	118.837 #
35) L7 AR-1260-5	8.542	7.445	573389	658137	130.451	113.601

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
Data File : P0069346.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2020 12:46
Operator : DD\AJ
Sample : L3157-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
CB-D35


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:47 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 13:50:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

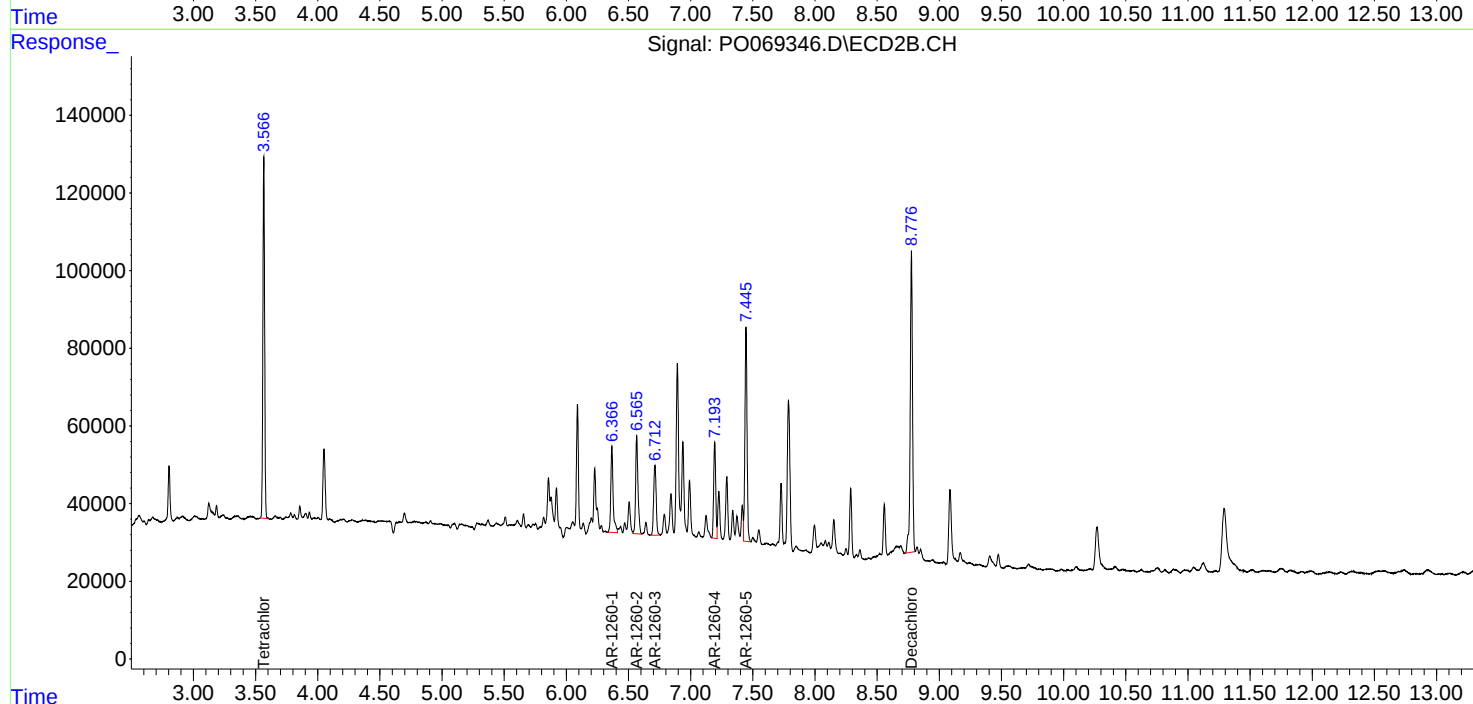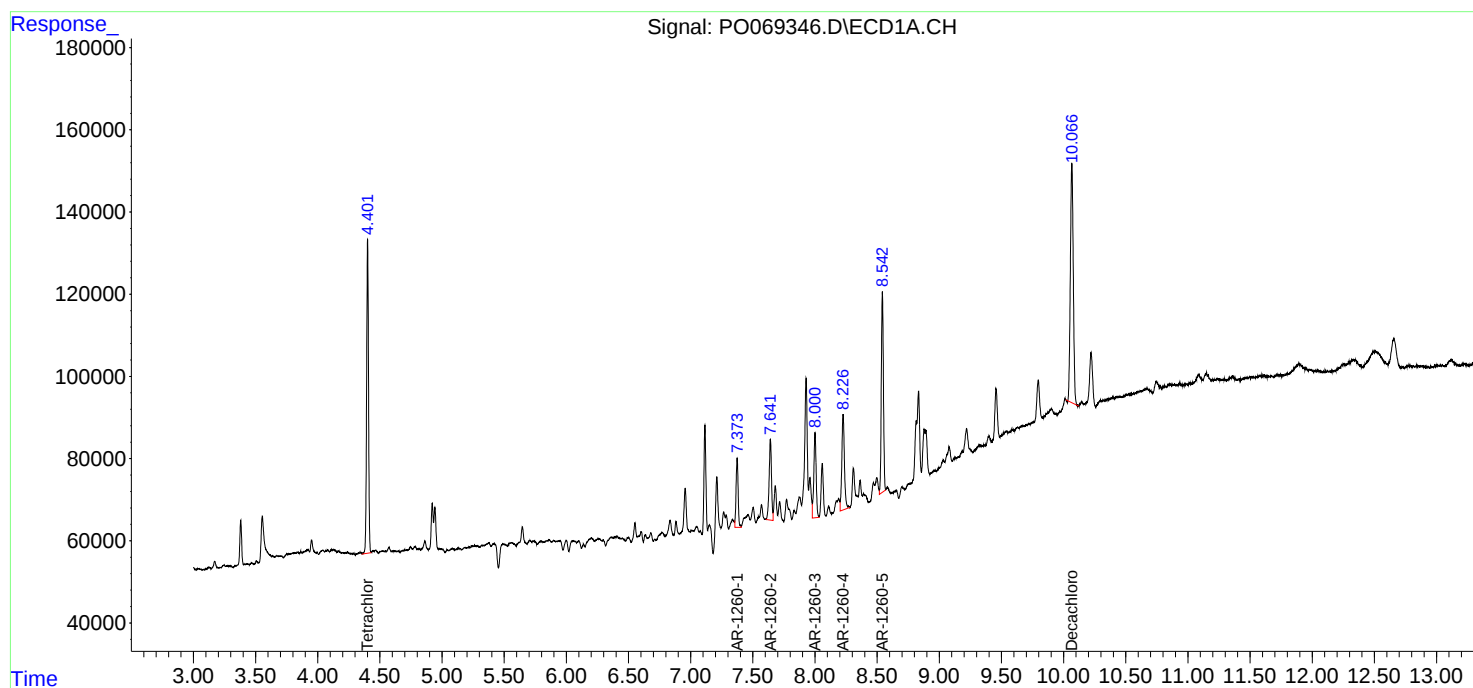

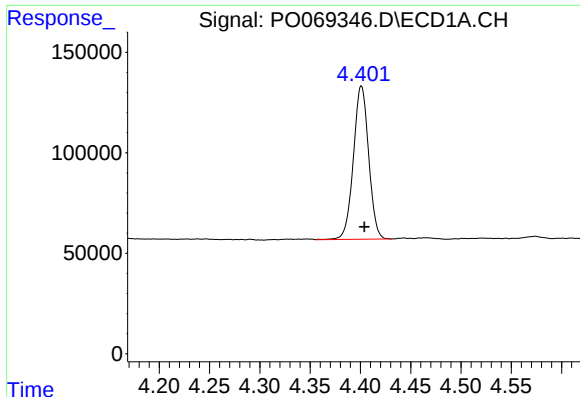


#1 Tetrachloro-m-xylene

R.T.: 4.401 min
Delta R.T.: -0.003 min
Response: 804741
Conc: 27.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-D35


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:47 AM

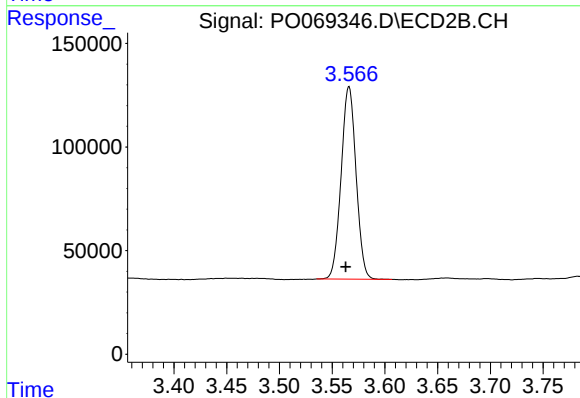


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.003 min
Response: 915549
Conc: 23.79 ng/ml

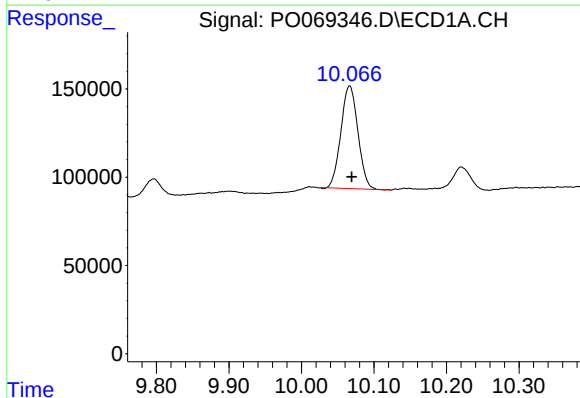


#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.003 min
Response: 947483
Conc: 19.95 ng/ml

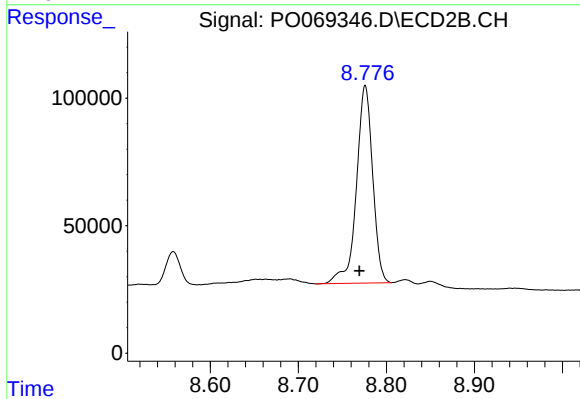

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.007 min
Response: 993743
Conc: 18.26 ng/ml

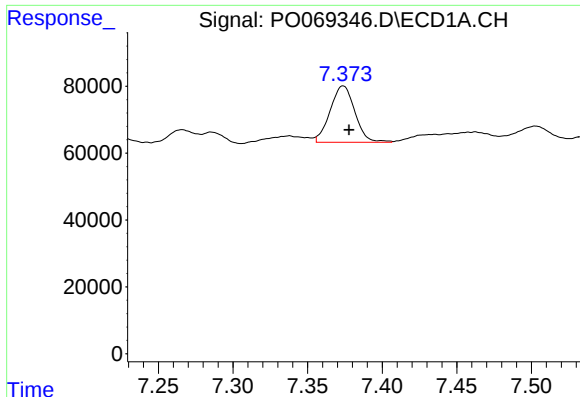


#31 AR-1260-1

R.T.: 7.373 min
Delta R.T.: -0.004 min
Response: 194466
Conc: 101.90 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CB-D35


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:47 AM

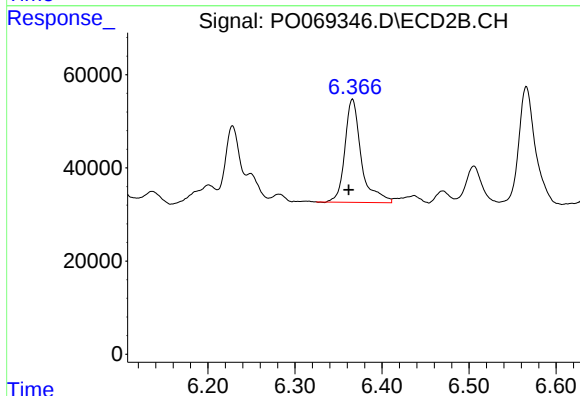


#31 AR-1260-1

R.T.: 6.366 min
Delta R.T.: 0.004 min
Response: 290020
Conc: 123.94 ng/ml

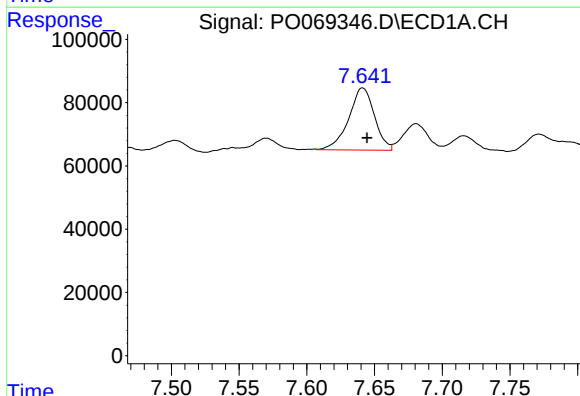


#32 AR-1260-2

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 260041
Conc: 111.10 ng/ml

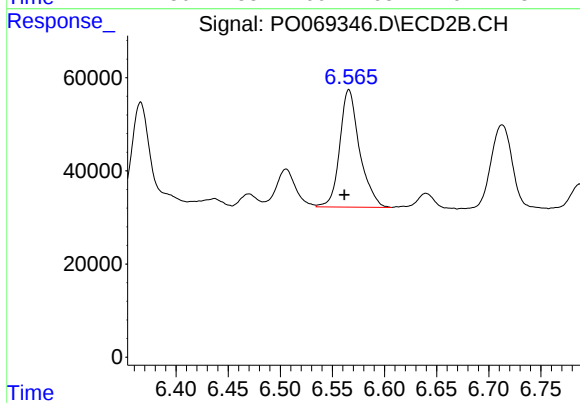

#32 AR-1260-2

R.T.: 6.566 min
Delta R.T.: 0.004 min
Response: 333805
Conc: 117.27 ng/ml

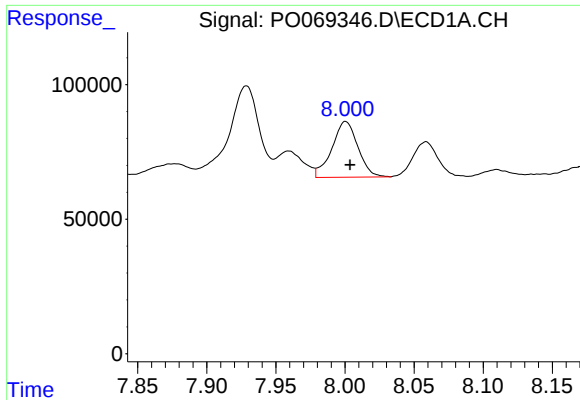


#33 AR-1260-3

R.T.: 8.001 min
Delta R.T.: -0.003 min
Response: 272145
Conc: 153.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-D35


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:47 AM

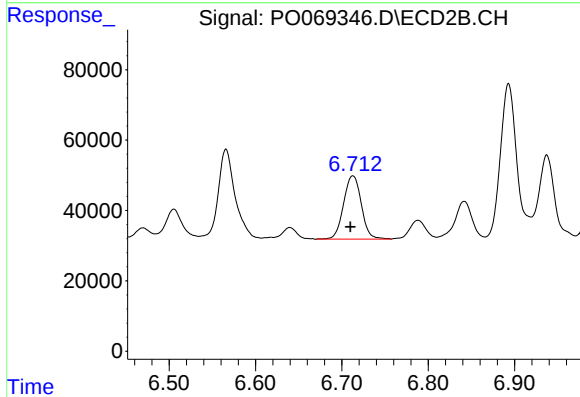


#33 AR-1260-3

R.T.: 6.713 min
Delta R.T.: 0.003 min
Response: 255970
Conc: 95.17 ng/ml

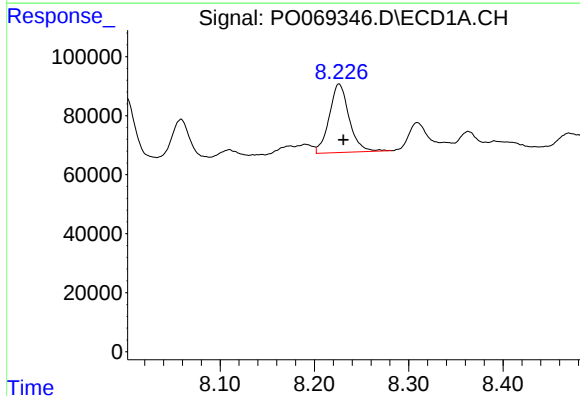


#34 AR-1260-4

R.T.: 8.226 min
Delta R.T.: -0.005 min
Response: 339328
Conc: 162.71 ng/ml

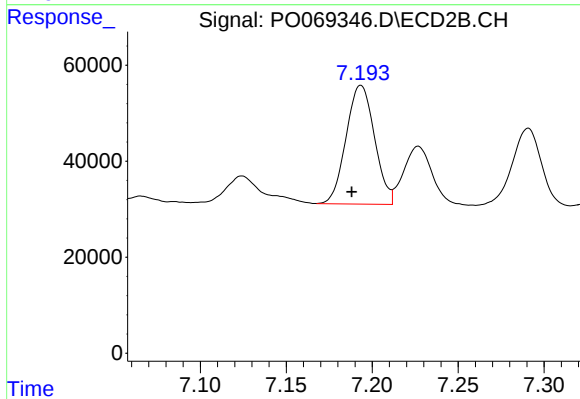

#34 AR-1260-4

R.T.: 7.193 min
Delta R.T.: 0.005 min
Response: 284718
Conc: 118.84 ng/ml

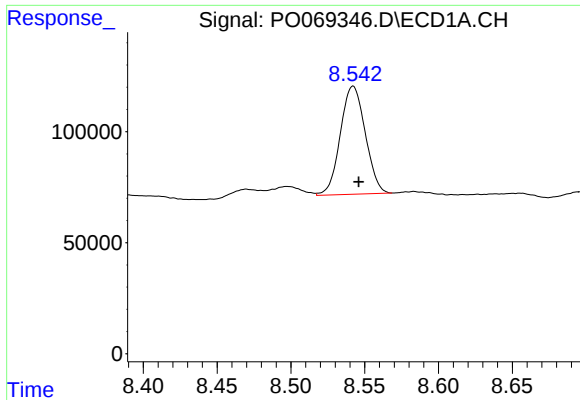


#35 AR-1260-5

R.T.: 8.542 min
Delta R.T.: -0.004 min
Response: 573389
Conc: 130.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-D35

Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:47 AM

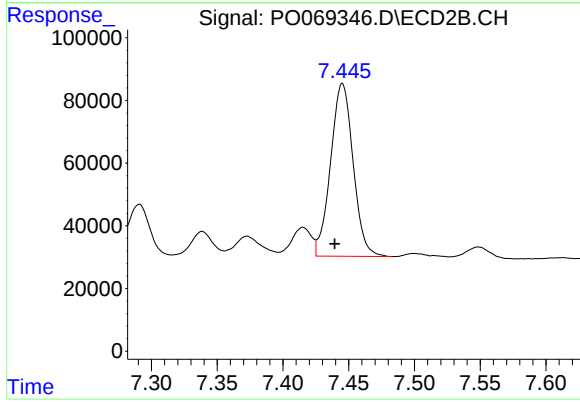

#35 AR-1260-5

R.T.: 7.445 min
Delta R.T.: 0.006 min
Response: 658137
Conc: 113.60 ng/ml