

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
 Data File : P0069347.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2020 13:03
 Operator : DD\AJ
 Sample : L3157-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CB-D40

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 13:50:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.565	831643	953964	28.112	24.785
2) SA Decachlor...	10.064	8.776	1063356	1122322	22.388	20.617

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
Data File : P0069347.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2020 13:03
Operator : DD\AJ
Sample : L3157-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
CB-D40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 13:50:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

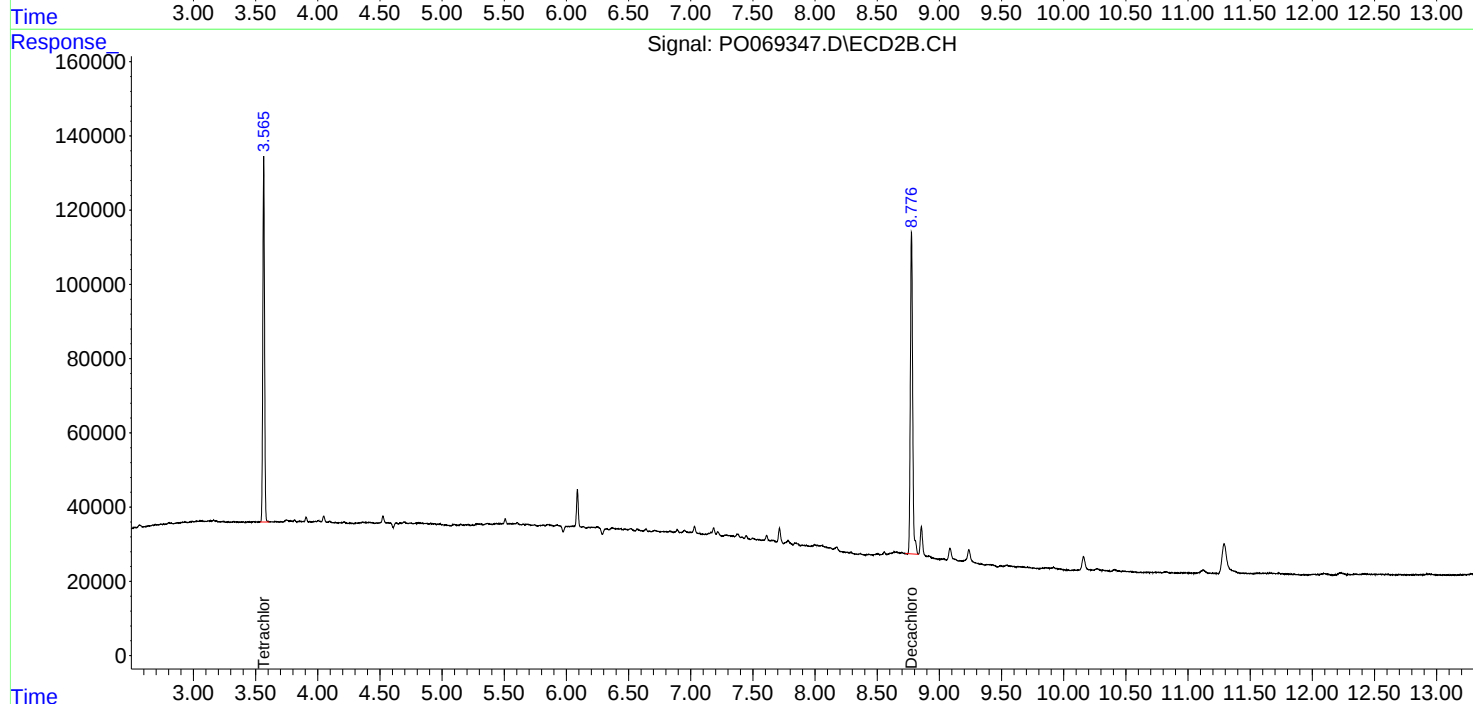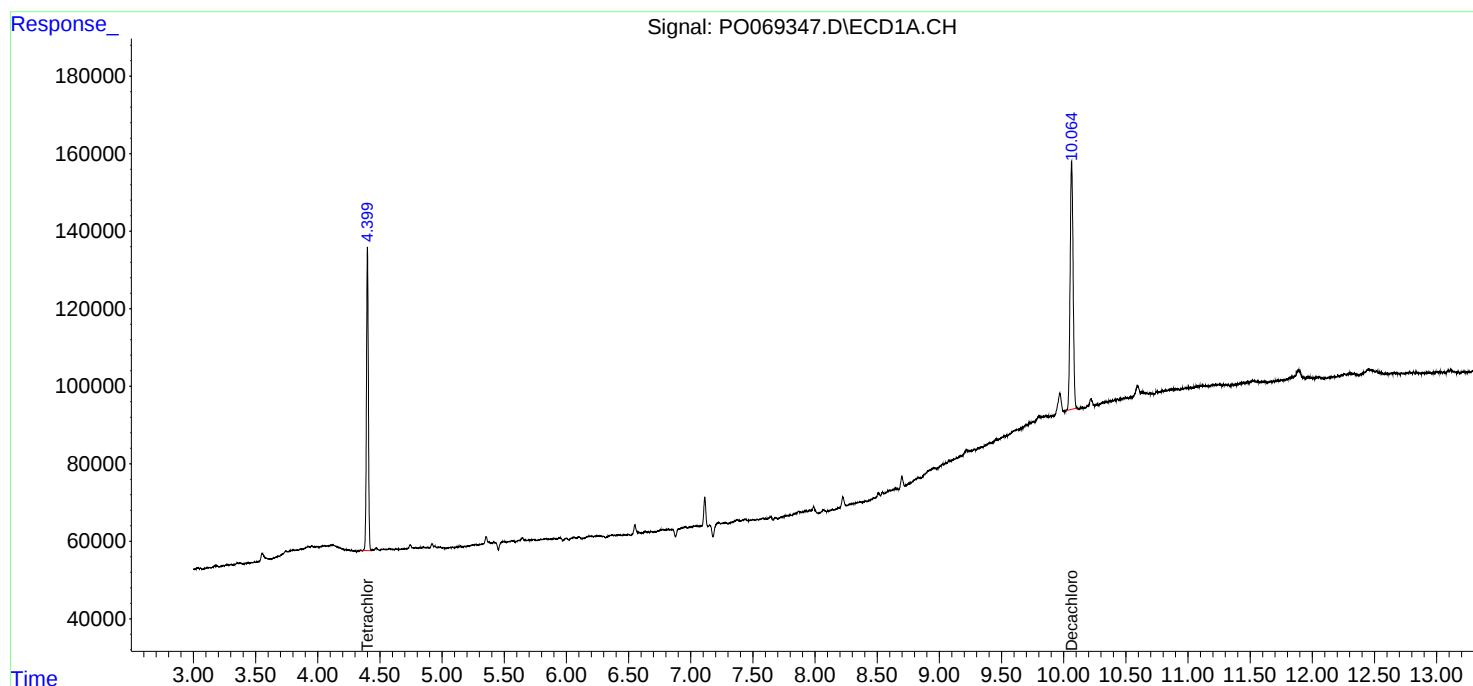


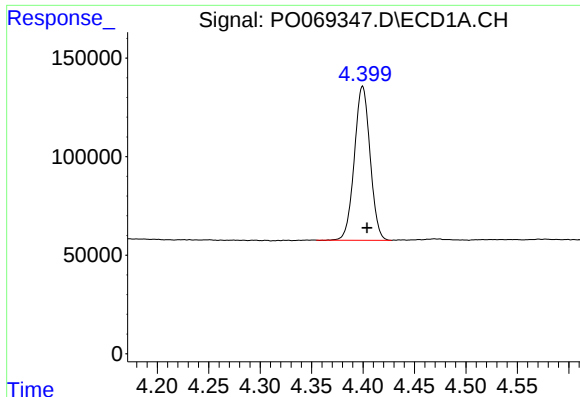

#1 Tetrachloro-m-xylene


R.T.: 4.400 min
Delta R.T.: -0.004 min
Response: 831643
Conc: 28.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
CB-D40

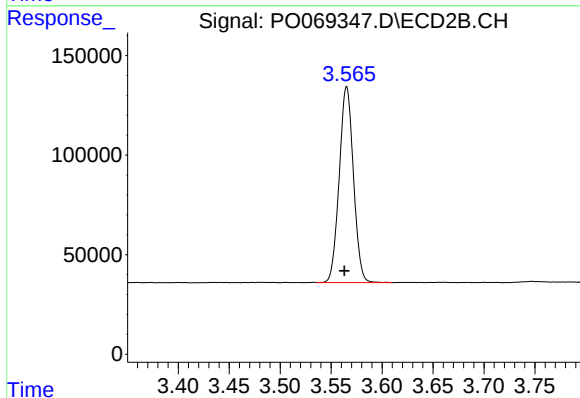


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.002 min
Response: 953964
Conc: 24.79 ng/ml

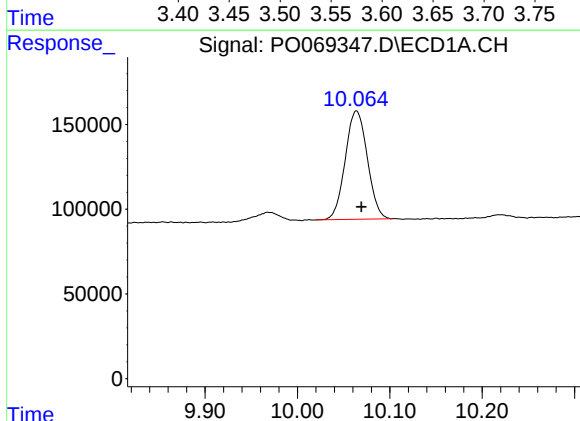

#2 Decachlorobiphenyl

R.T.: 10.064 min
Delta R.T.: -0.005 min
Response: 1063356
Conc: 22.39 ng/ml

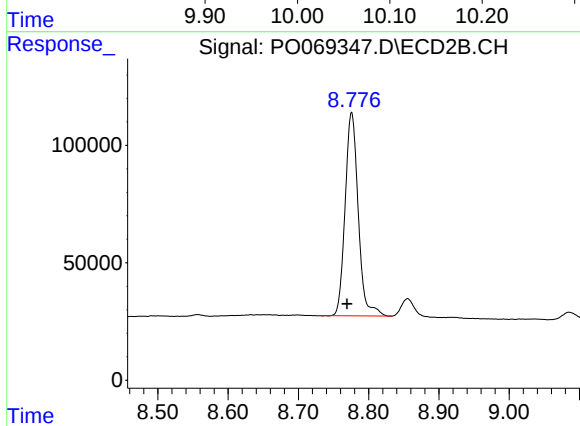

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.006 min
Response: 1122322
Conc: 20.62 ng/ml