

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
 Data File : P0069350.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Jul 2020 13:54
 Operator : DD\AJ
 Sample : L3162-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GL-SP

Manual Integrations
 APPROVED

Ankita
 7/2/2020 10:44:51 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 14:50:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.565	884788	1016356	29.908	26.406m
2) SA Decachlor...	10.063	8.776	1152862	1082566	24.273m	19.887

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070120\
Data File : P0069350.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Jul 2020 13:54
Operator : DD\AJ
Sample : L3162-02
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
GL-SP


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:51 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 14:50:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

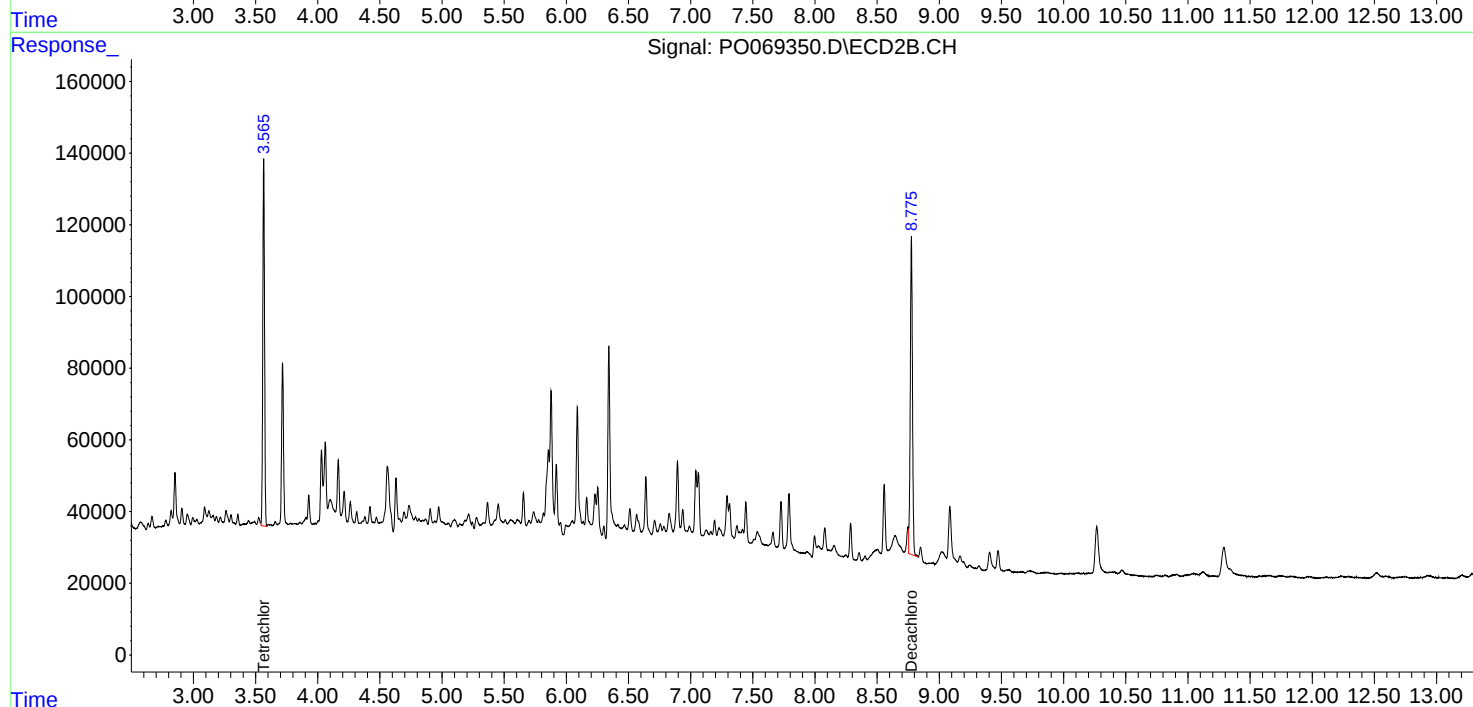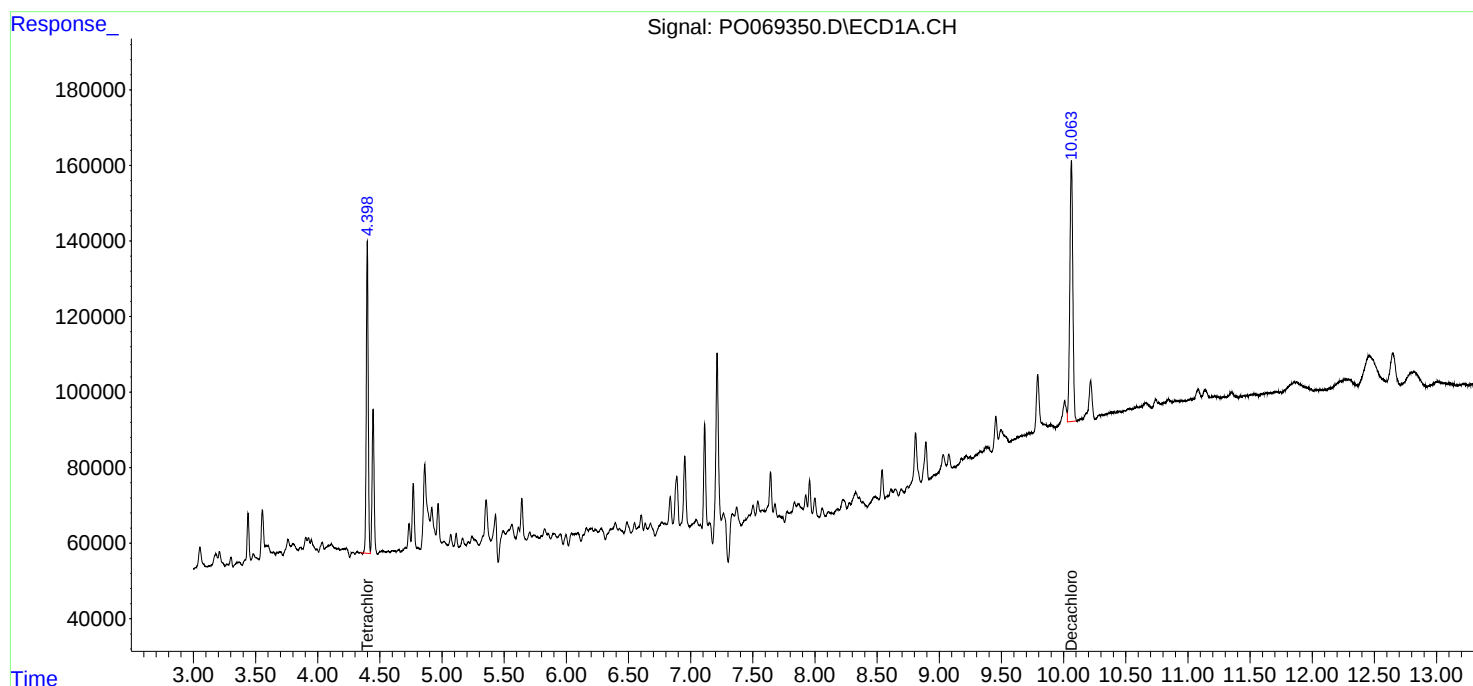

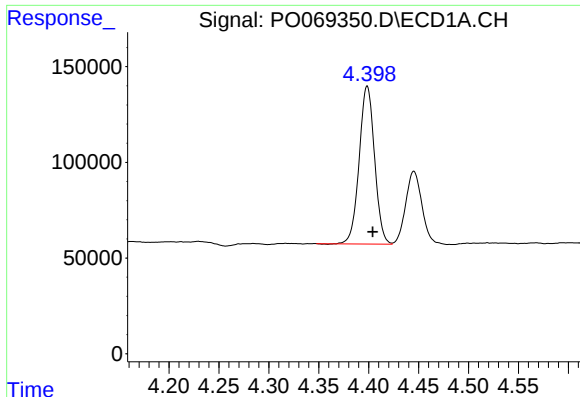


#1 Tetrachloro-m-xylene

R.T.: 4.399 min
Delta R.T.: -0.005 min
Response: 884788
Conc: 29.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
GL-SP


Manual Integrations
APPROVED

Ankita
7/2/2020 10:44:51 AM

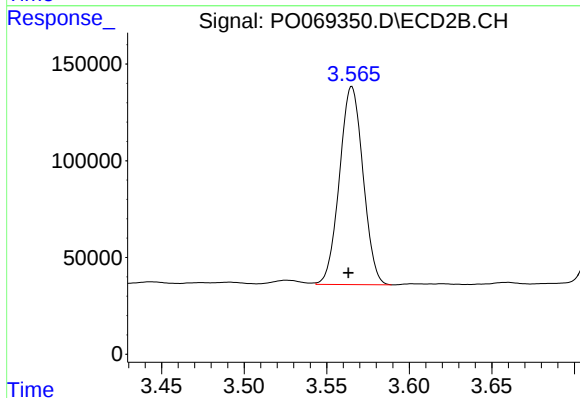


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.002 min
Response: 1016356
Conc: 26.41 ng/ml m

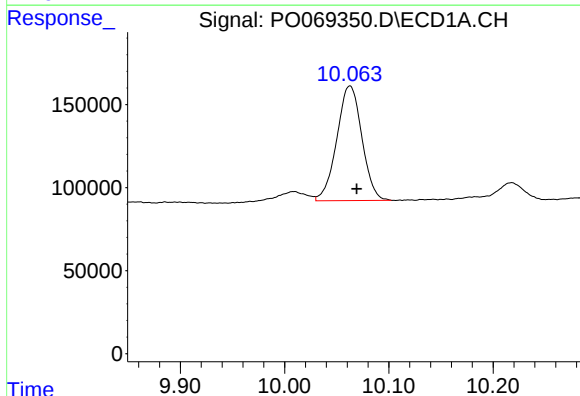

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.007 min
Response: 1152862
Conc: 24.27 ng/ml m

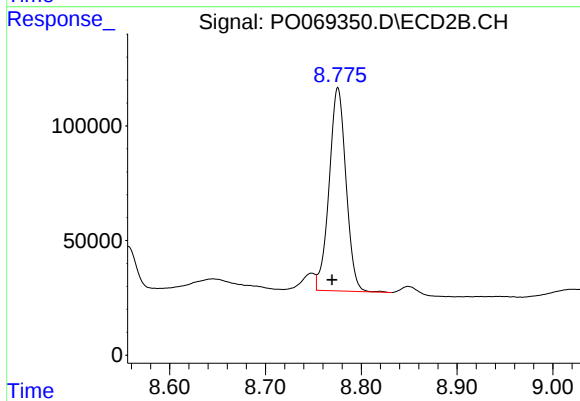

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.006 min
Response: 1082566
Conc: 19.89 ng/ml