

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070122\
 Data File : P0087713.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Jul 2022 16:14
 Operator : YP/AJ
 Sample : N3564-26
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 WC-16-2-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/05/2022
 Supervised By :Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 01 22:36:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.451	3.611	38317645	16202140	14.804	16.466
2) SA Decachlor...	10.305	8.628	62619391	64167231	30.656m	79.154m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070122\
Data File : PO087713.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Jul 2022 16:14
Operator : YP/AJ
Sample : N3564-26
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
WC-16-2-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 01 22:36:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

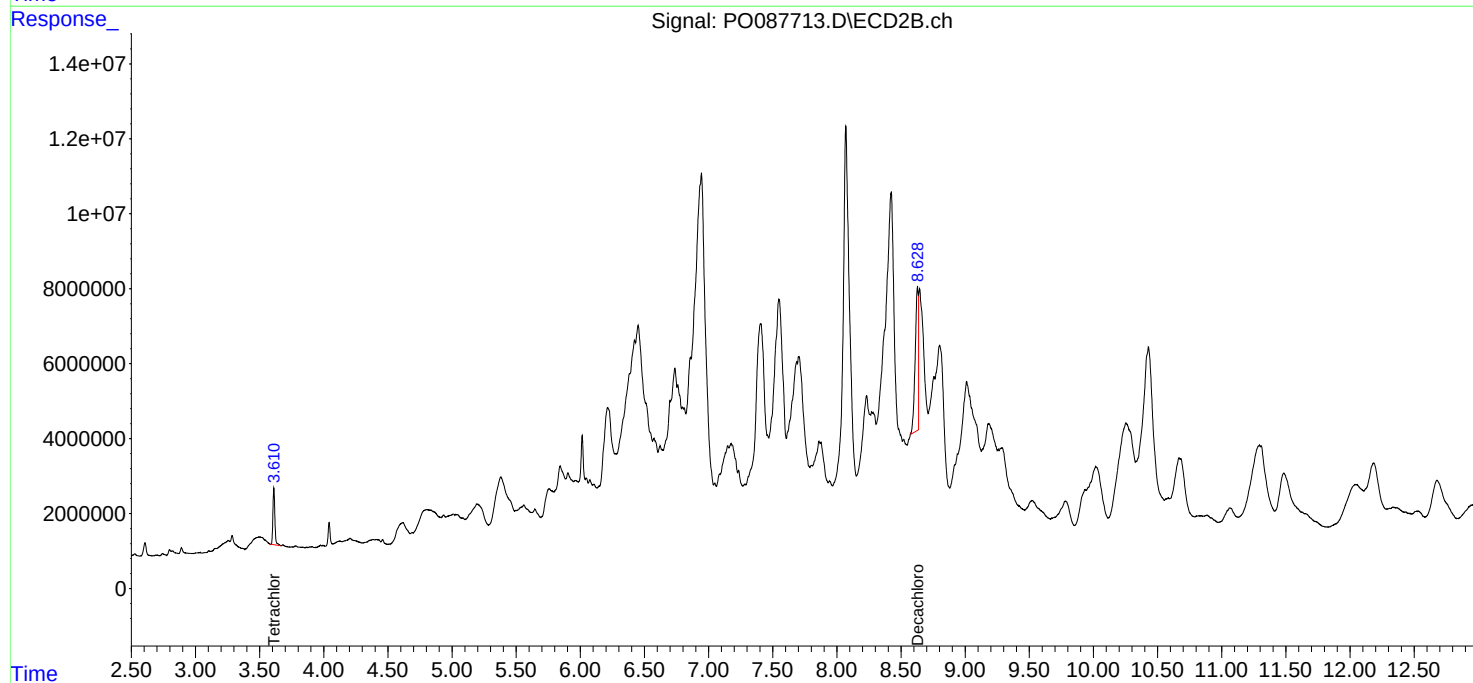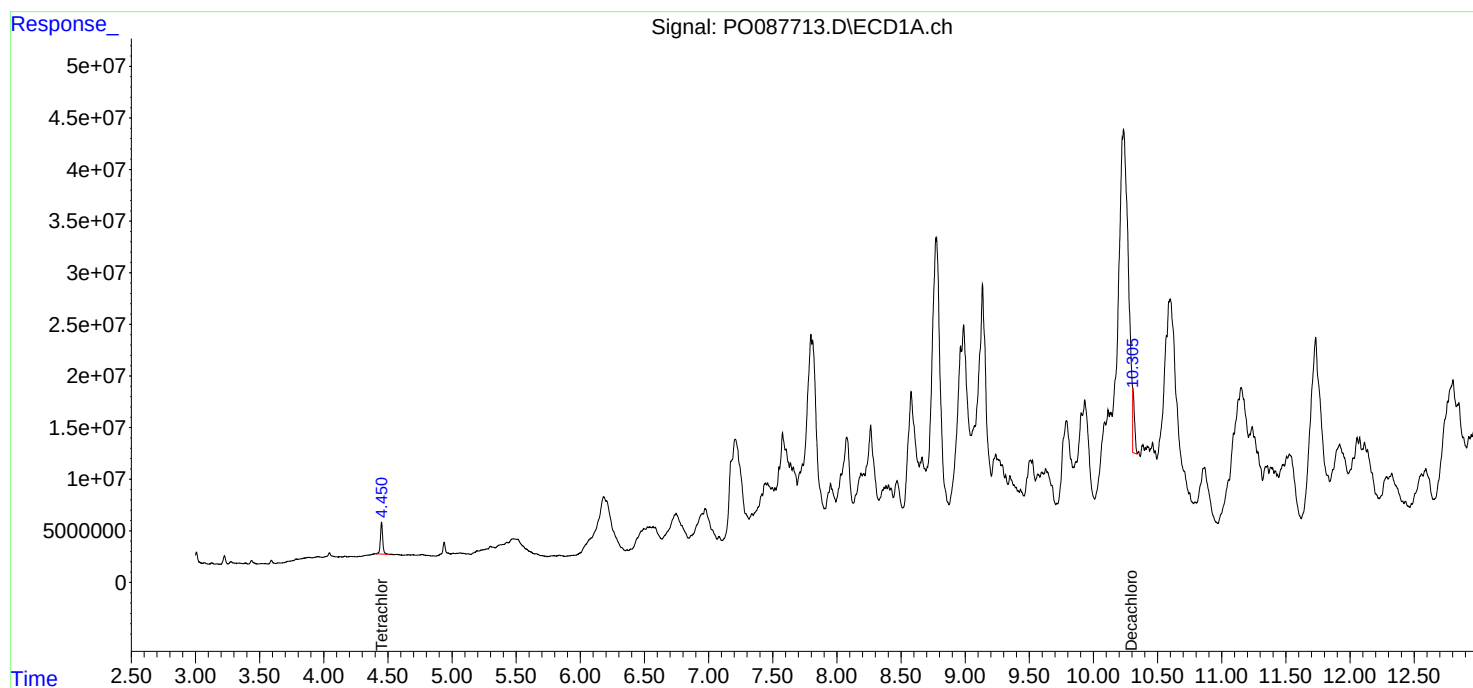

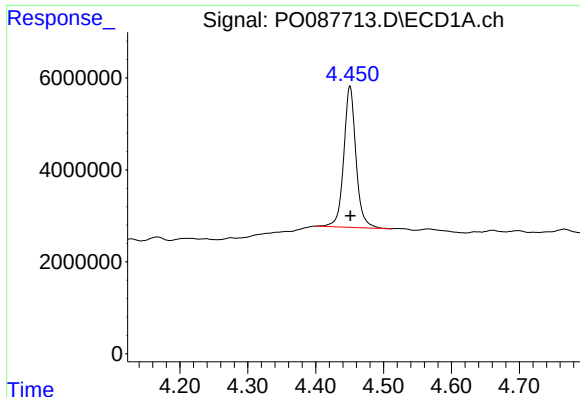


#1 Tetrachloro-m-xylene

R.T.: 4.451 min
Delta R.T.: 0.000 min
Response: 38317645
Conc: 14.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
WC-16-2-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/05/2022
Supervised By :Ankita Jodhani 07/05/2022

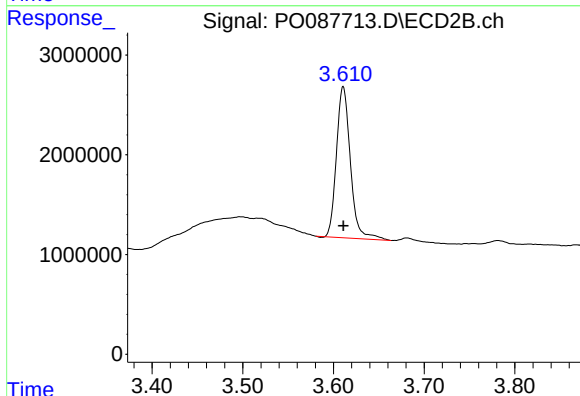


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.000 min
Response: 16202140
Conc: 16.47 ng/ml

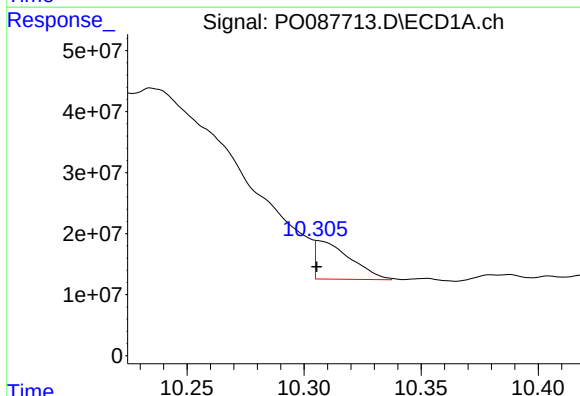

#2 Decachlorobiphenyl

R.T.: 10.305 min
Delta R.T.: 0.000 min
Response: 62619391
Conc: 30.66 ng/ml m

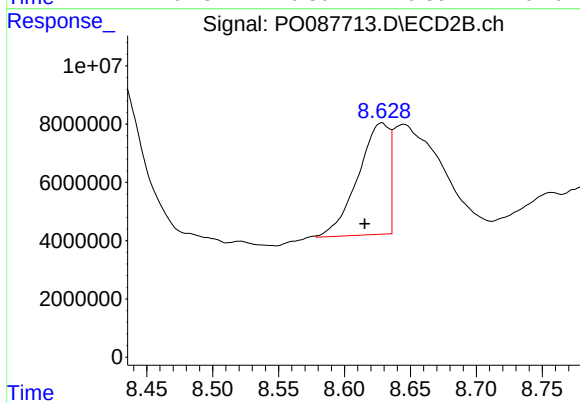

#2 Decachlorobiphenyl

R.T.: 8.628 min
Delta R.T.: 0.013 min
Response: 64167231
Conc: 79.15 ng/ml m