

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070125\
 Data File : P0111959.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 01:10
 Operator : YP/AJ
 Sample : Q2462-10 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 62725

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/02/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 03:16:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.675	3.672	10372479	8746955	1.801	1.557
2) SA Decachlor...	8.707	8.655	7183388	2700251	1.368	1.519m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070125\
Data File : PO111959.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 01:10
Operator : YP/AJ
Sample : Q2462-10 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
62725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/02/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 03:16:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

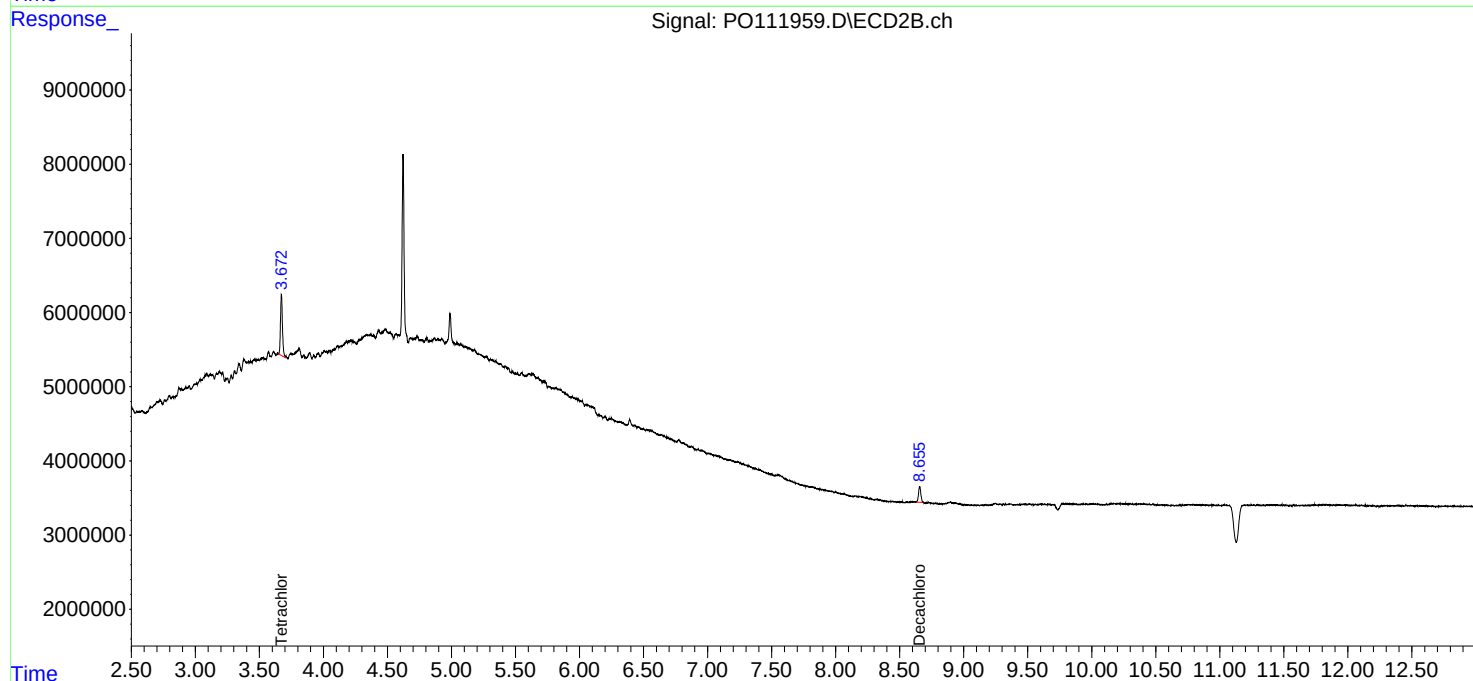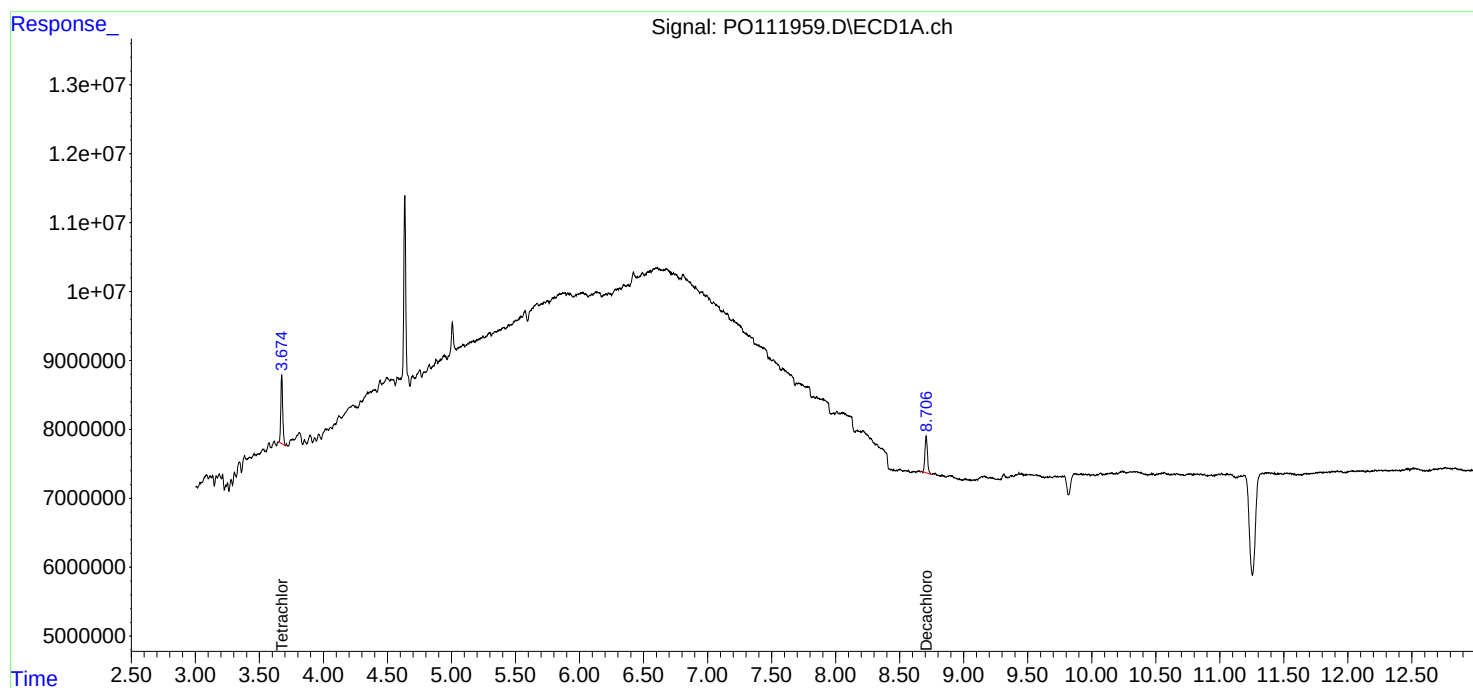

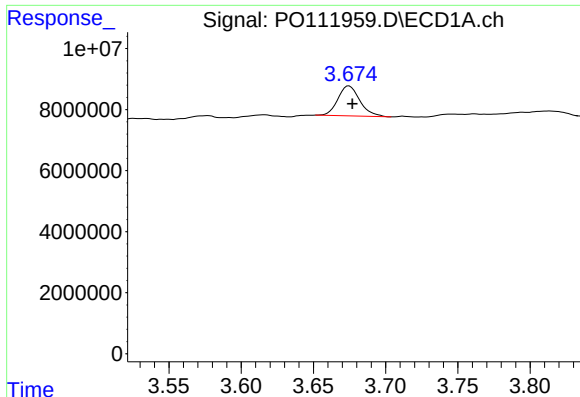


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.002 min
Response: 10372479
Conc: 1.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
62725


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/02/2025
Supervised By :mohammad ahmed 07/04/2025

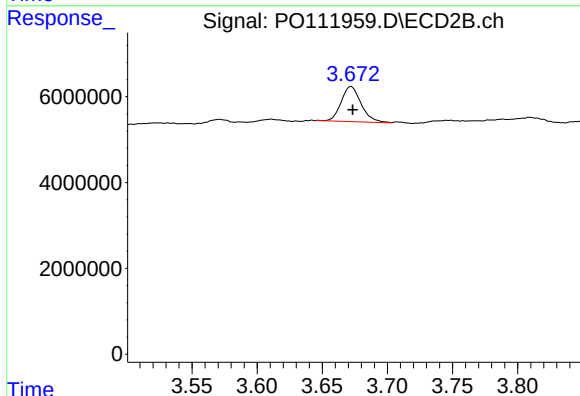


#1 Tetrachloro-m-xylene

R.T.: 3.672 min
Delta R.T.: -0.001 min
Response: 8746955
Conc: 1.56 ng/ml

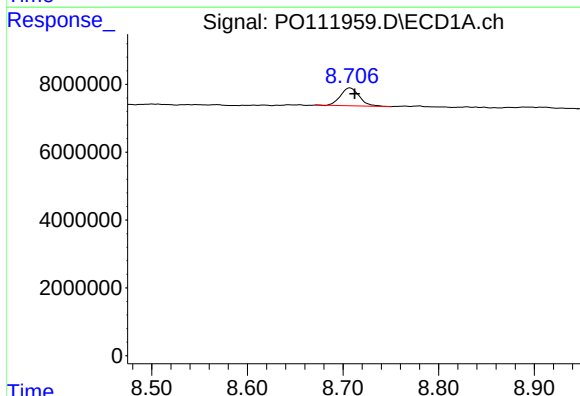

#2 Decachlorobiphenyl

R.T.: 8.707 min
Delta R.T.: -0.005 min
Response: 7183388
Conc: 1.37 ng/ml

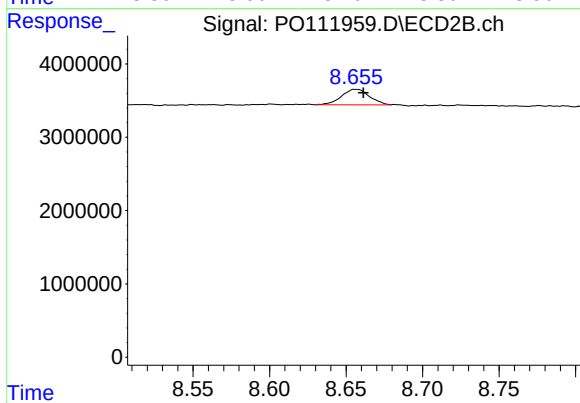

#2 Decachlorobiphenyl

R.T.: 8.655 min
Delta R.T.: -0.006 min
Response: 2700251
Conc: 1.52 ng/ml m