

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
 Data File : P0046434.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2018 13:37
 Operator : SM/UA
 Sample : J3806-01 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A464262

Manual Integrations
 APPROVED

Sohil
 7/9/2018 8:30:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 14:35:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 02 12:59:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.375	3.610	298687	514654	1.068m	4.894m#
2) SA Decachlor...	10.040	8.565	629566	195367	2.361m	2.134m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
Data File : P0046434.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2018 13:37
Operator : SM/UA
Sample : J3806-01 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A464262


Manual Integrations
APPROVED

Sohil
7/9/2018 8:30:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 14:35:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 02 12:59:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

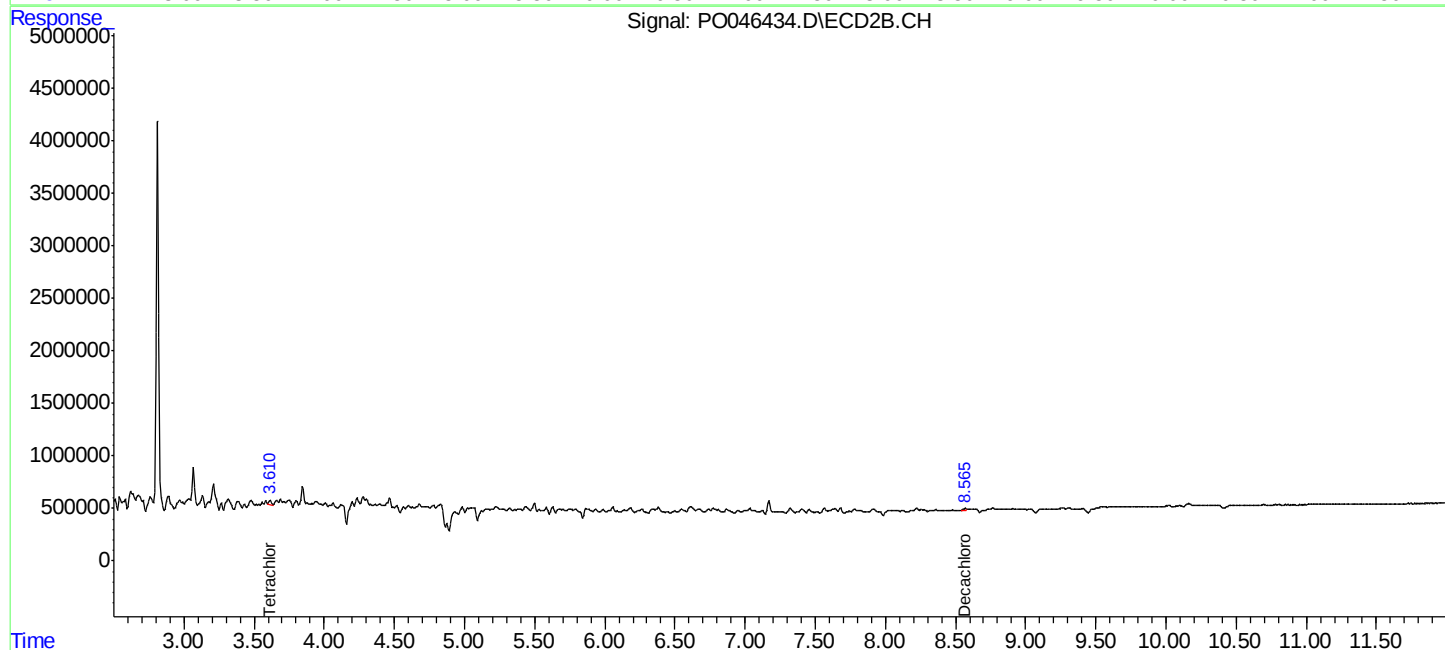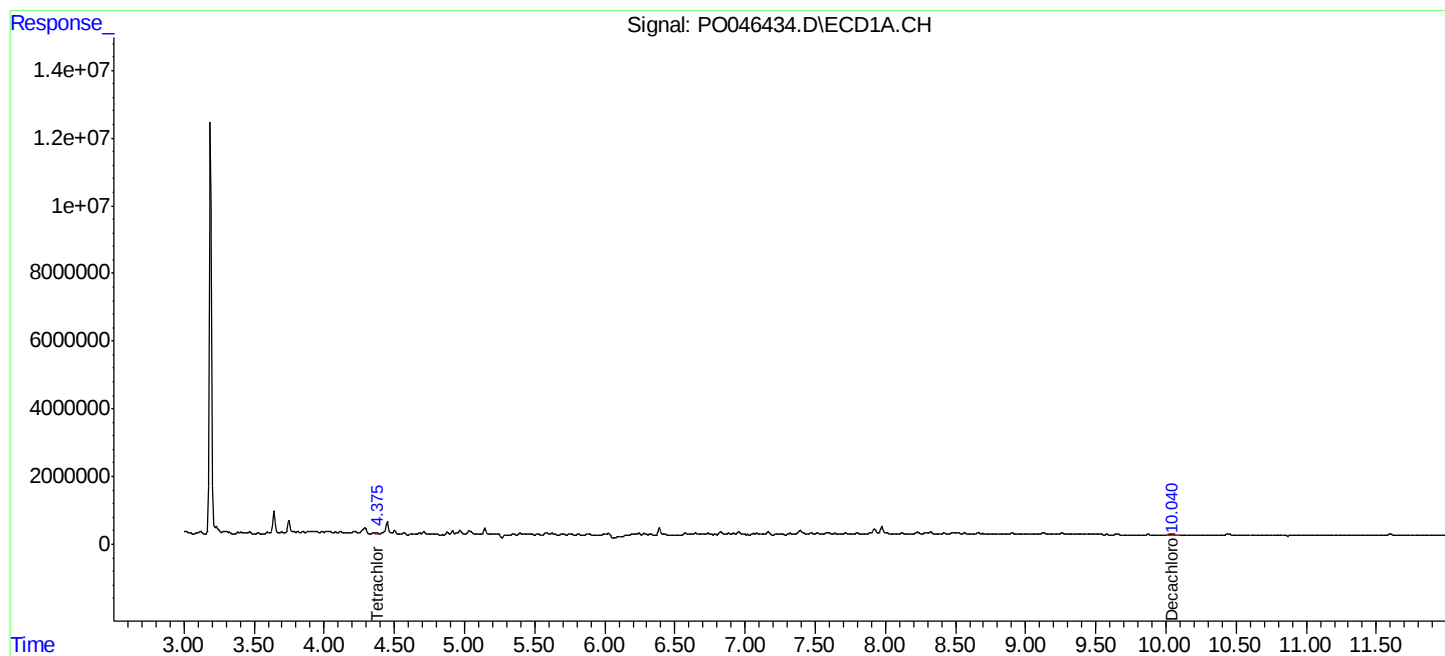

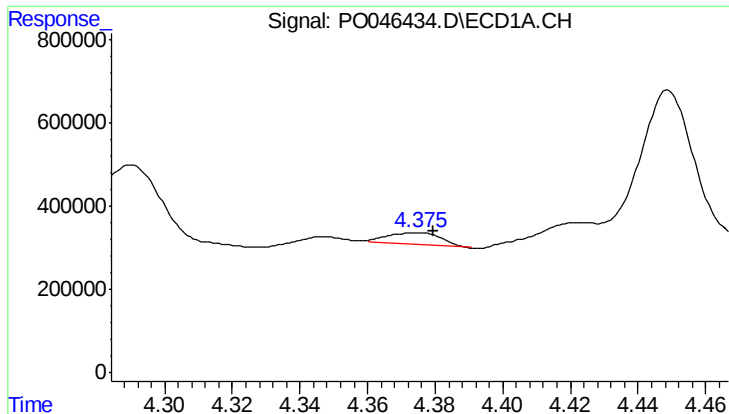


#1 Tetrachloro-m-xylene

R.T.: 4.375 min
Delta R.T.: -0.004 min
Response: 298687
Conc: 1.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
A464262


Manual Integrations
APPROVED

Sohil
7/9/2018 8:30:36 AM

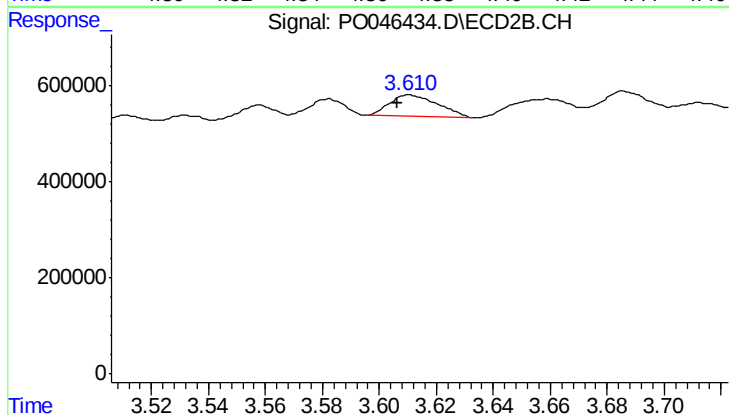


#1 Tetrachloro-m-xylene

R.T.: 3.610 min
Delta R.T.: 0.004 min
Response: 514654
Conc: 4.89 ng/ml m

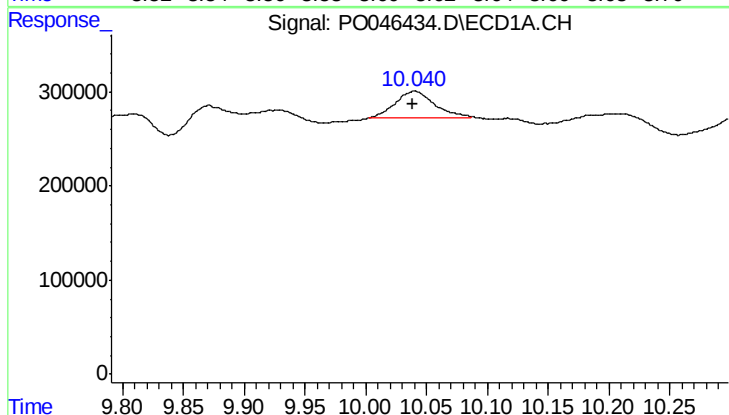

#2 Decachlorobiphenyl

R.T.: 10.040 min
Delta R.T.: 0.002 min
Response: 629566
Conc: 2.36 ng/ml m

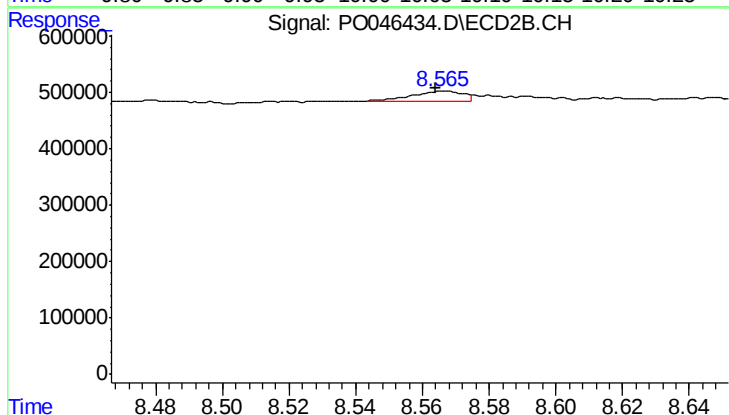

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: 0.001 min
Response: 195367
Conc: 2.13 ng/ml m