

Data Path : Z:\bestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
 Data File : P0046435.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2018 13:53
 Operator : SM/UA
 Sample : J3806-02 10X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B464329

Manual Integrations
 APPROVED

Sohil
 7/9/2018 8:30:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 16:15:57 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jul 02 12:59:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	nq/ml	nq/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.376	3.611	459042	646457	1.642m	6.148m#
2) SA Decachlor...	10.039	8.568	499230	113426	1.872m	1.239m#

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
Data File : P0046435.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2018 13:53
Operator : SM/UA
Sample : J3806-02 10X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
B464329


Manual Integrations
APPROVED

Sohil
7/9/2018 8:30:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 16:15:57 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 02 12:59:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

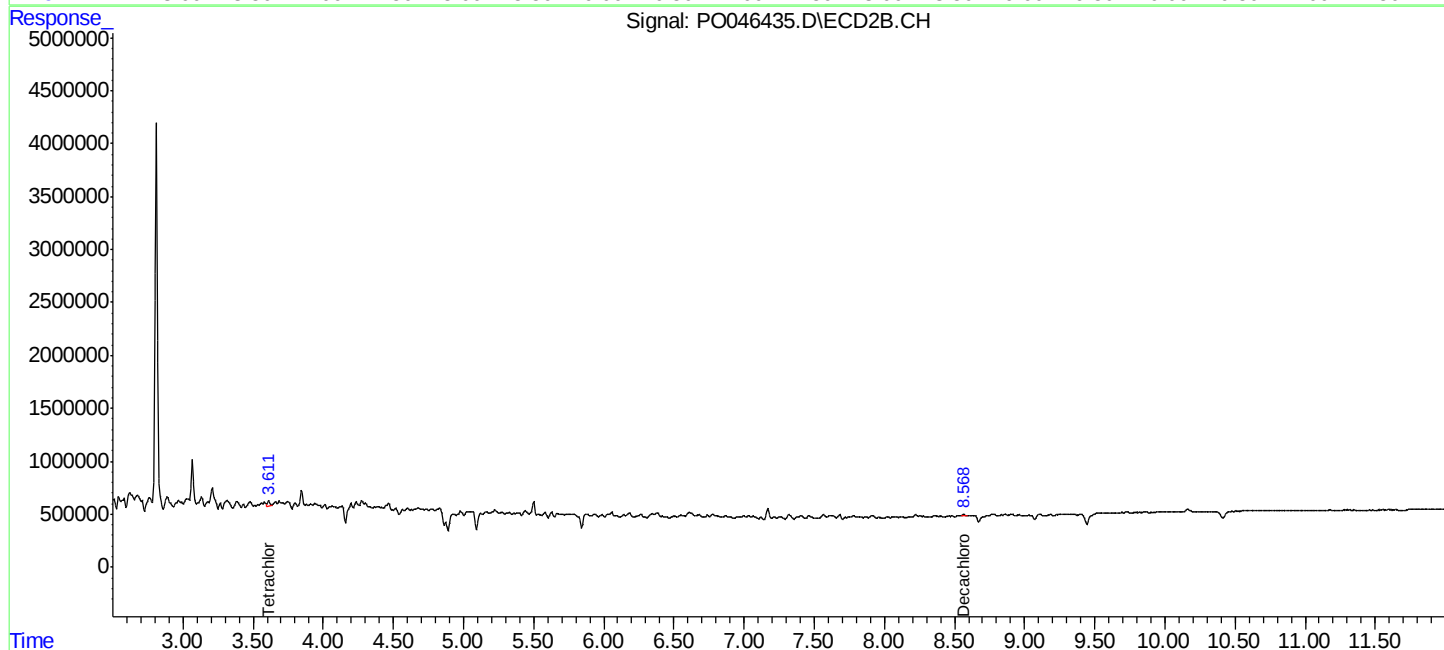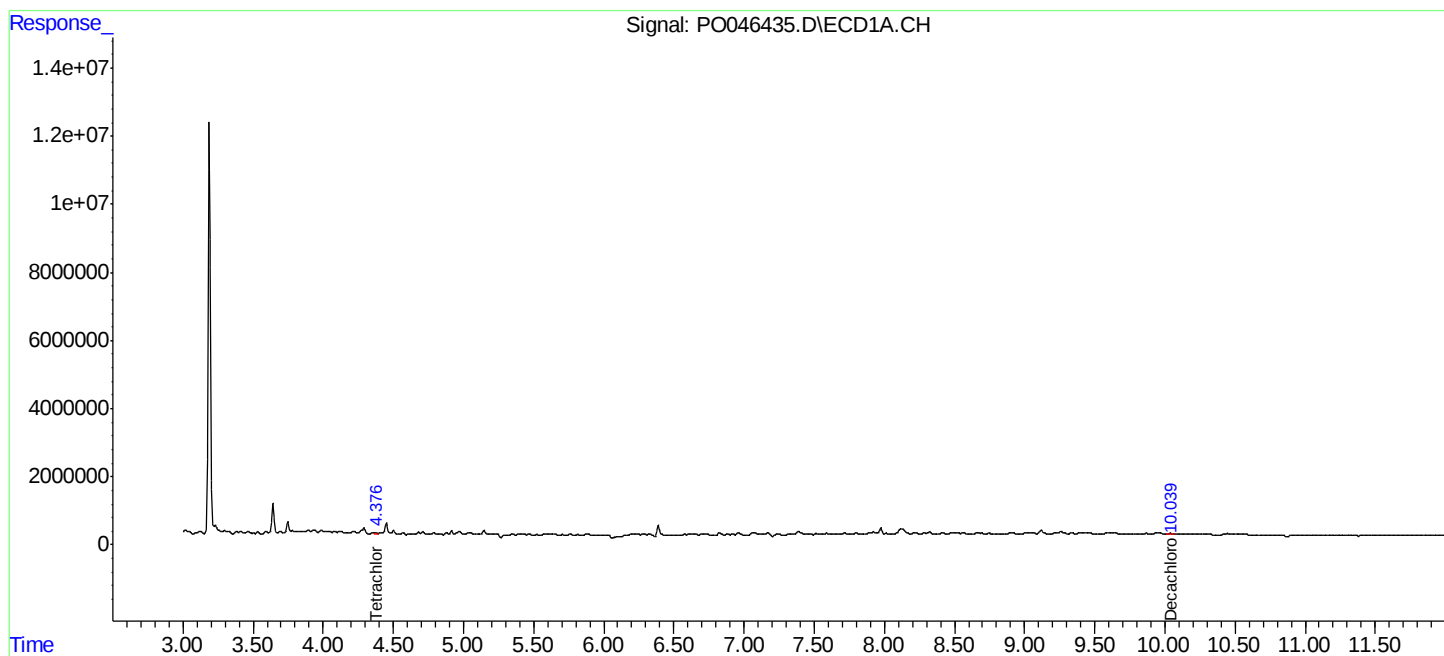

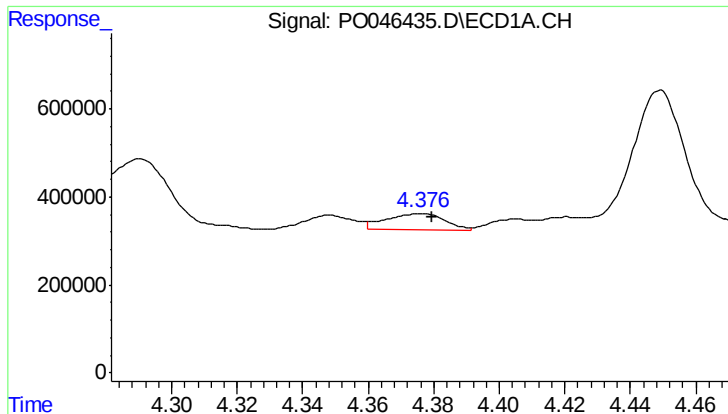


#1 Tetrachloro-m-xylene

R.T.: 4.376 min
Delta R.T.: -0.004 min
Response: 459042
Conc: 1.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
B464329


Manual Integrations
APPROVED

Sohil
7/9/2018 8:30:37 AM

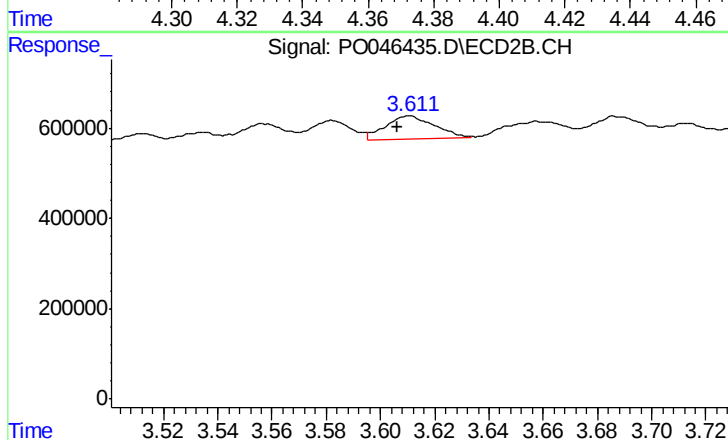


#1 Tetrachloro-m-xylene

R.T.: 3.611 min
Delta R.T.: 0.004 min
Response: 646457
Conc: 6.15 ng/ml m

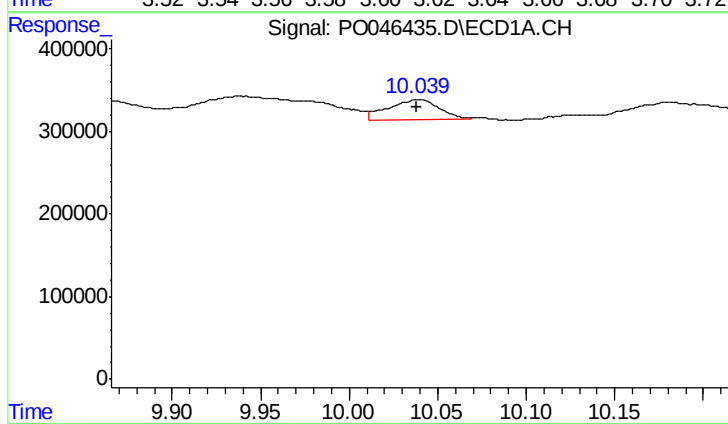

#2 Decachlorobiphenyl

R.T.: 10.039 min
Delta R.T.: 0.000 min
Response: 499230
Conc: 1.87 ng/ml m

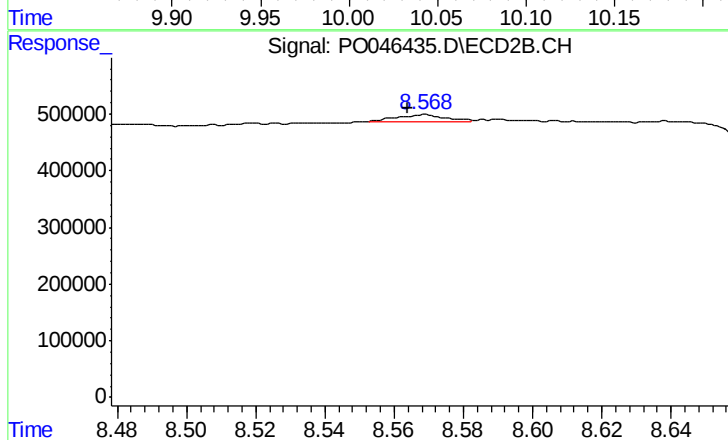

#2 Decachlorobiphenyl

R.T.: 8.568 min
Delta R.T.: 0.004 min
Response: 113426
Conc: 1.24 ng/ml m