

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
Data File : P0046439.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2018 14:57
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 15:10:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 02 12:59:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.607	7137854	3002167	25.532	28.549
2) SA Decachlor...	10.037	8.563	5719072	1933119	21.448	21.111

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD 0\Data\P0070218\
Data File : P0046439.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2018 14:57
Operator : SM/UA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 15:10:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 02 12:59:36 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Ini. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

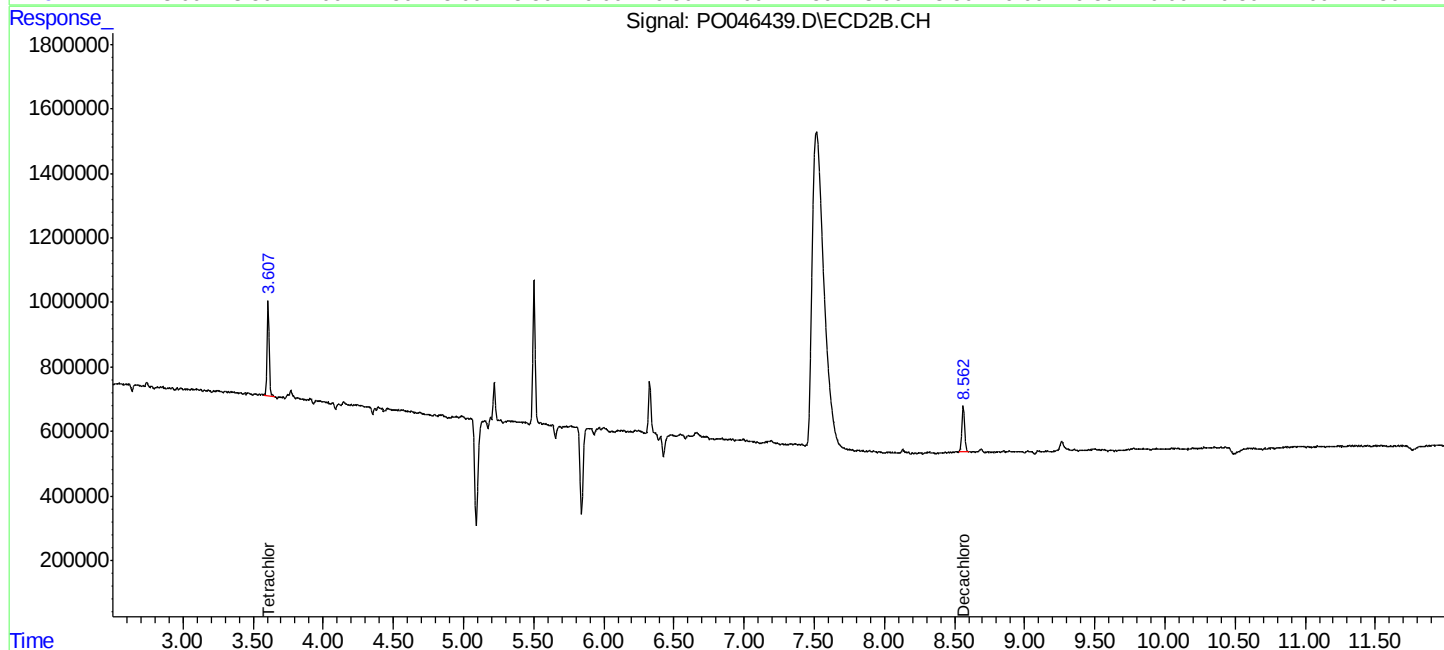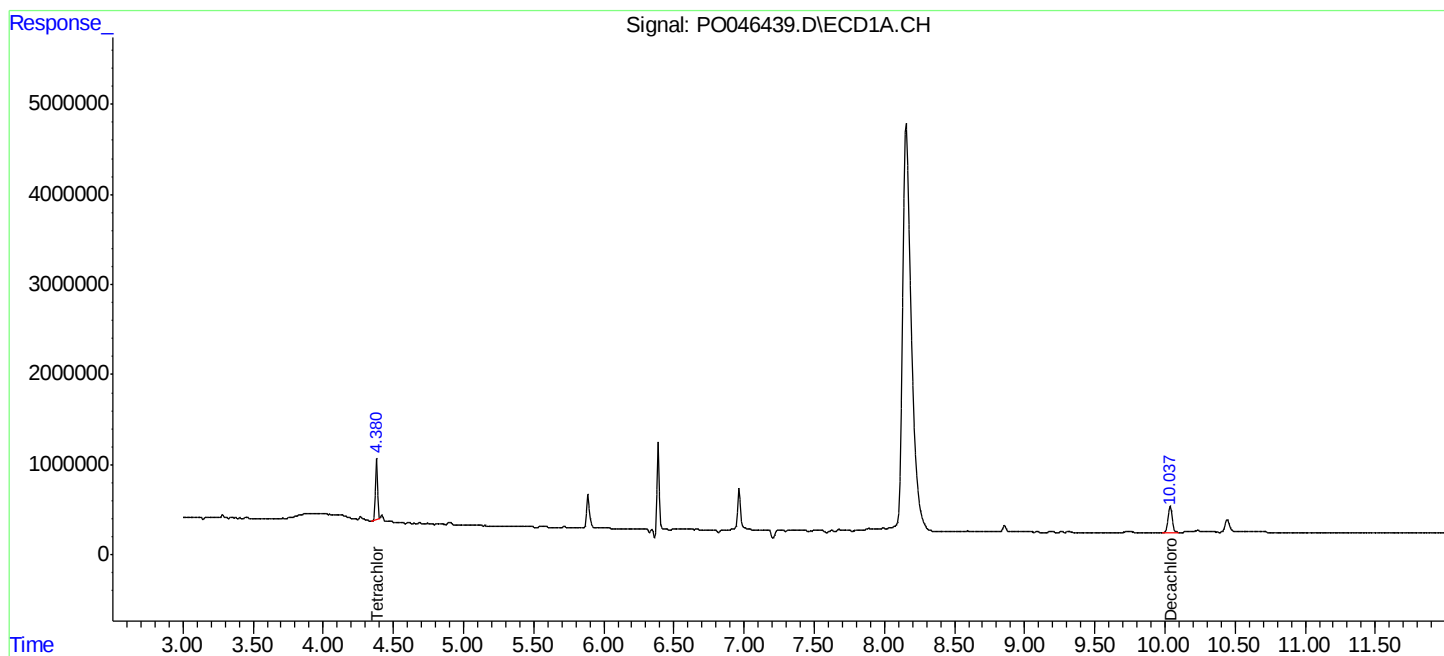


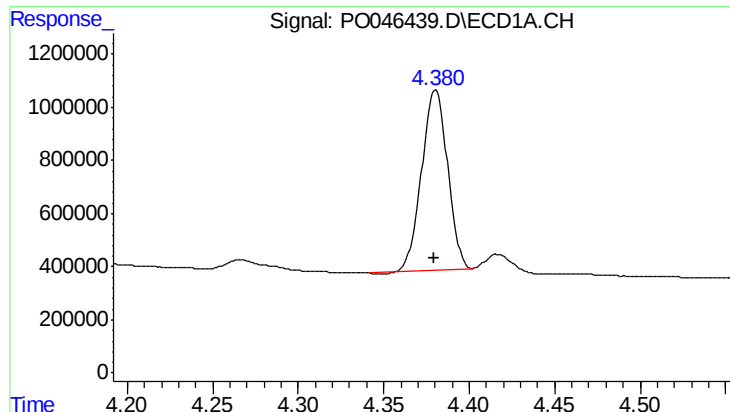

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: 0.000 min
Response: 7137854
Conc: 25.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

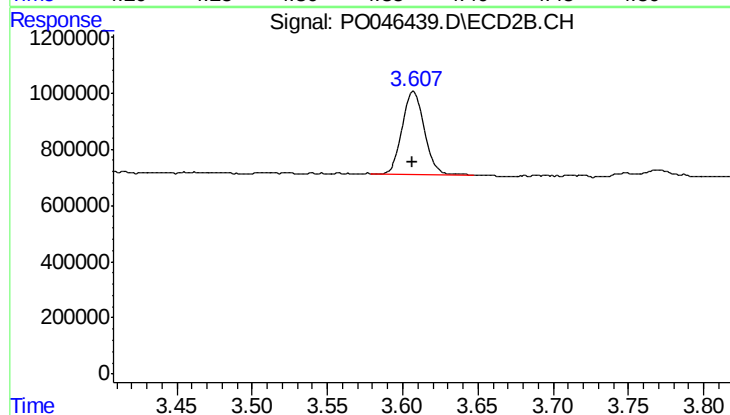


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: 0.000 min
Response: 3002167
Conc: 28.55 ng/ml

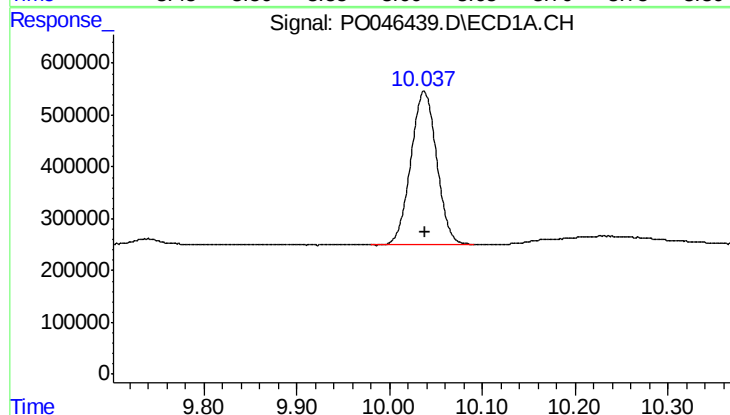

#2 Decachlorobiphenyl

R.T.: 10.037 min
Delta R.T.: -0.001 min
Response: 5719072
Conc: 21.45 ng/ml

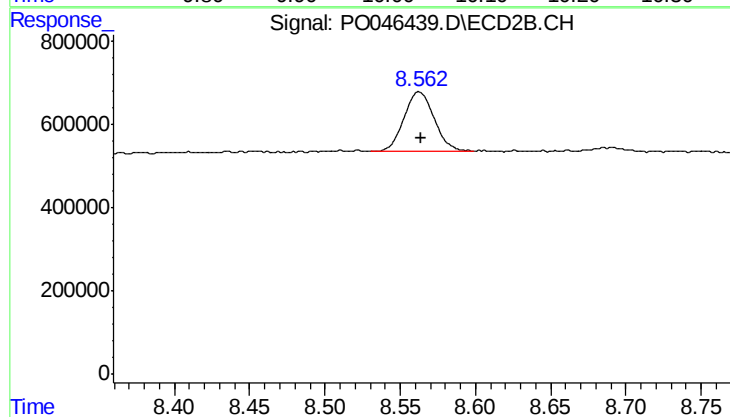

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.001 min
Response: 1933119
Conc: 21.11 ng/ml