

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070219\
 Data File : P0057671.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2019 13:25
 Operator : SM/SJ
 Sample : K3526-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 13:45:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 24 14:02:43 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.216	3.546	761044	688875	19.374	19.591
2) SA Decachlor...	9.754	8.461	1065884	679862	18.955	18.175
Target Compounds						
27) L6 AR-1254-2	0.000	5.614	0	53084	N.D.	28.520 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070219\
Data File : P0057671.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2019 13:25
Operator : SM/SJ
Sample : K3526-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 13:45:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062419.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 24 14:02:43 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

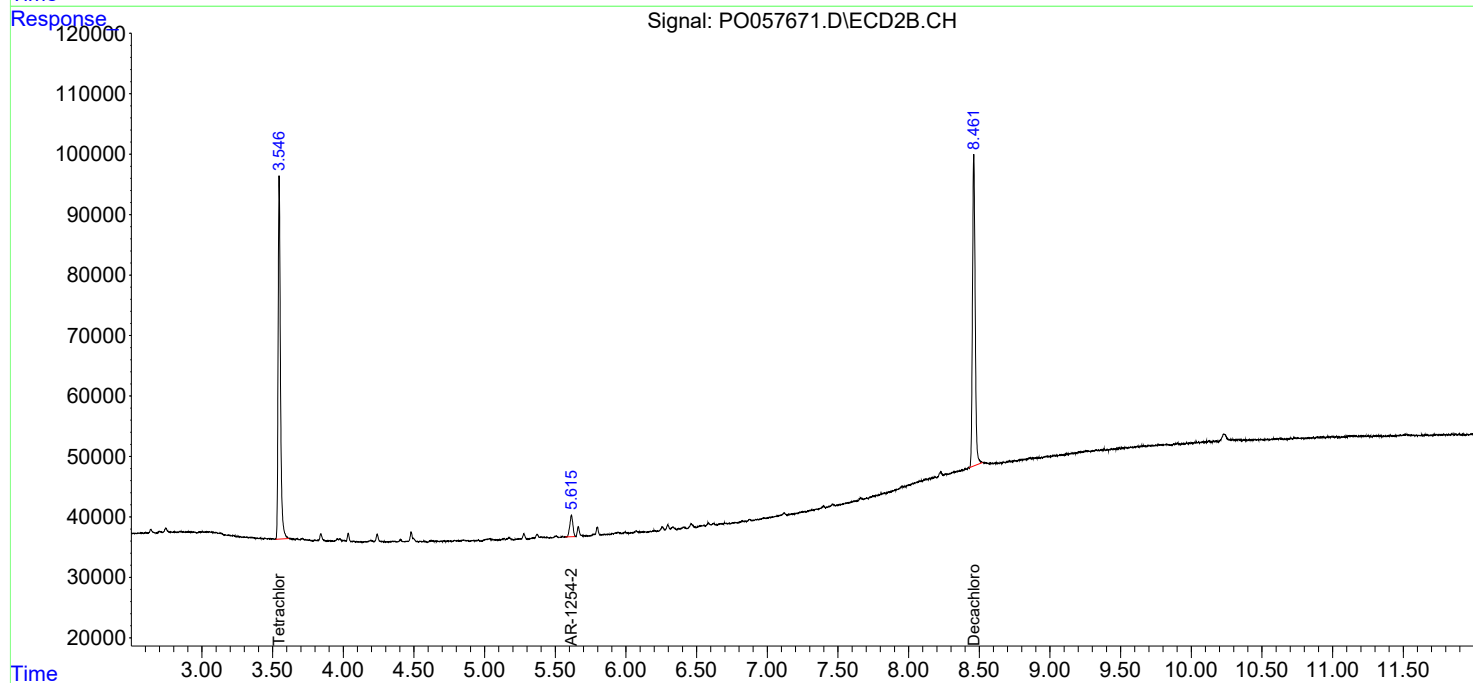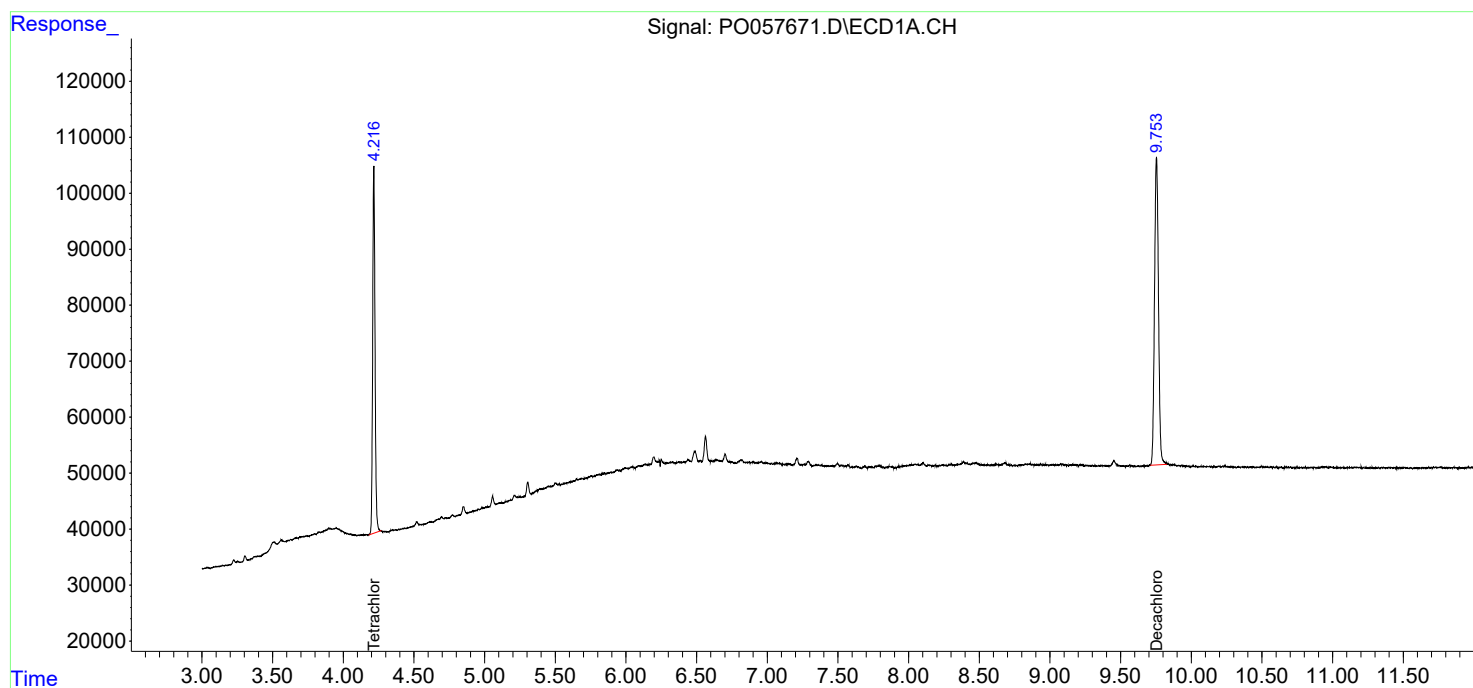


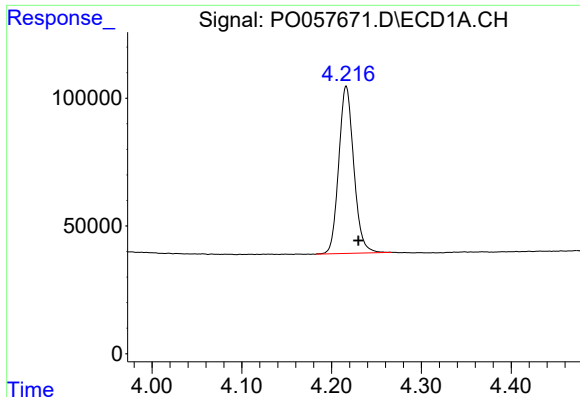

#1 Tetrachloro-m-xylene


R.T.: 4.216 min
Delta R.T.: -0.014 min
Response: 761044
Conc: 19.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP

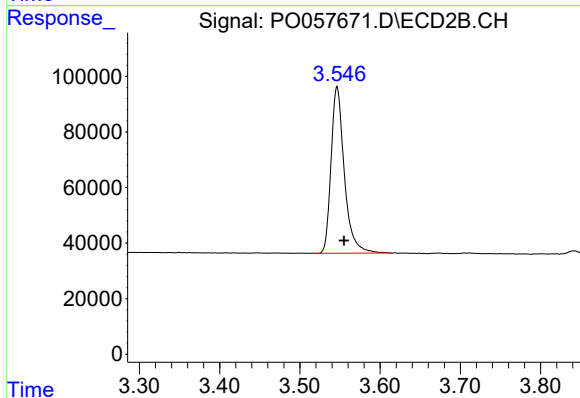


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: -0.009 min
Response: 688875
Conc: 19.59 ng/ml

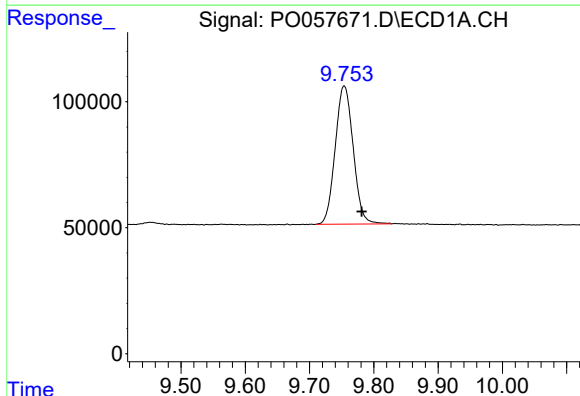


#2 Decachlorobiphenyl

R.T.: 9.754 min
Delta R.T.: -0.027 min
Response: 1065884
Conc: 18.95 ng/ml

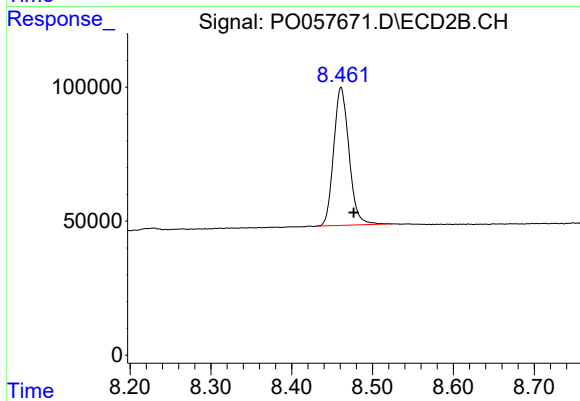

#2 Decachlorobiphenyl


R.T.: 8.461 min
Delta R.T.: -0.016 min
Response: 679862
Conc: 18.17 ng/ml

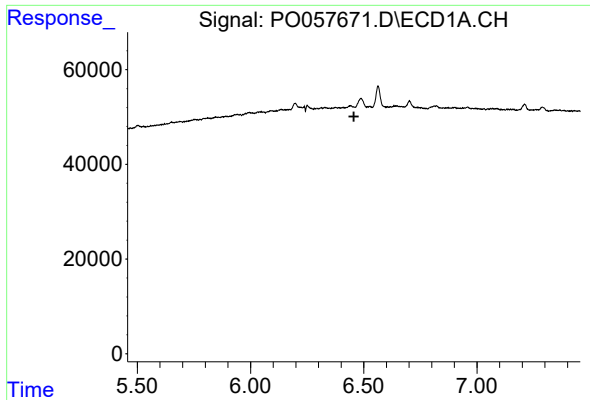

#27 AR-1254-2

R.T.: 0.000 min
Exp R.T.: 6.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
SB-03-COMP

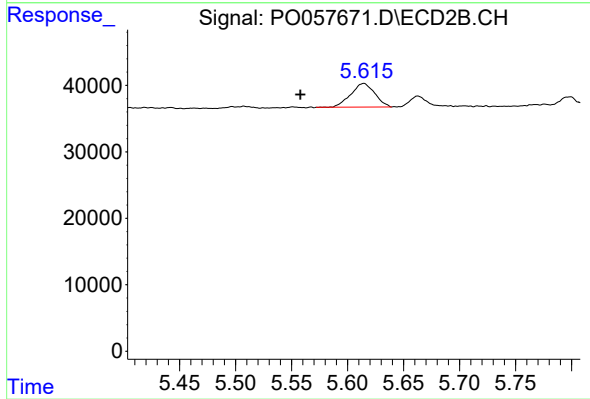

#27 AR-1254-2

R.T.: 5.614 min
Delta R.T.: 0.056 min
Response: 53084
Conc: 28.52 ng/ml