

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070220\
 Data File : P0069359.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Jul 2020 10:08
 Operator : DD\AJ
 Sample : L3126-11
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-4-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 02 10:29:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.566	1020398	1117497	34.493	29.034
2) SA Decachlor...	10.062	8.776	1105139	1066165	23.268	19.586

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070220\
Data File : P0069359.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Jul 2020 10:08
Operator : DD\AJ
Sample : L3126-11
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-4-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 02 10:29:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

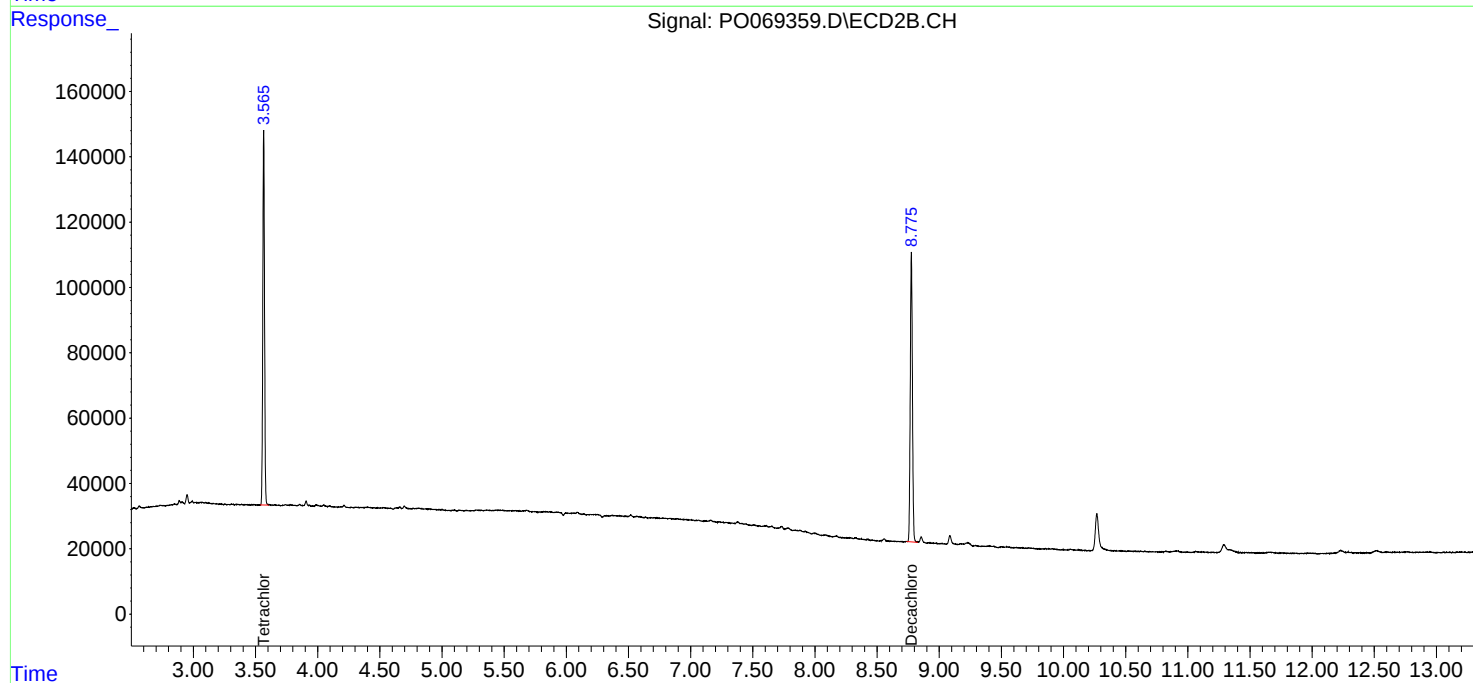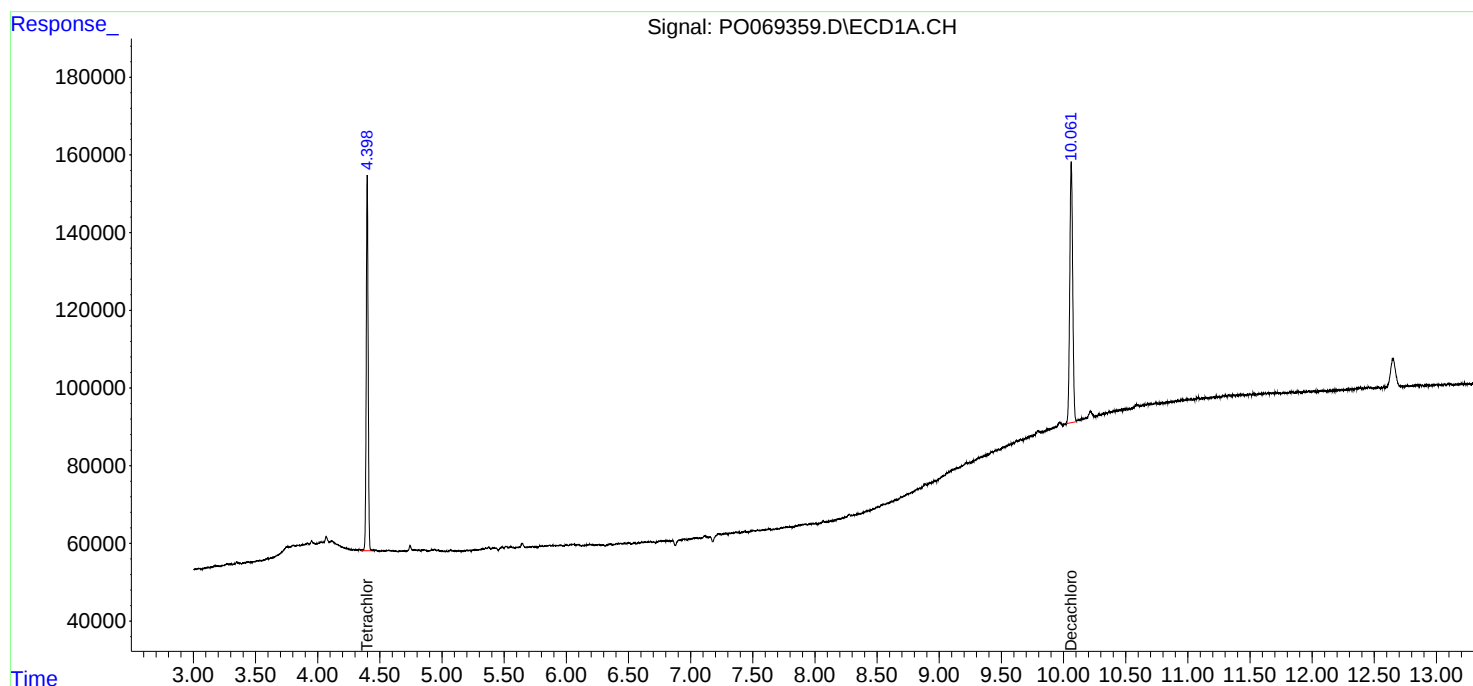


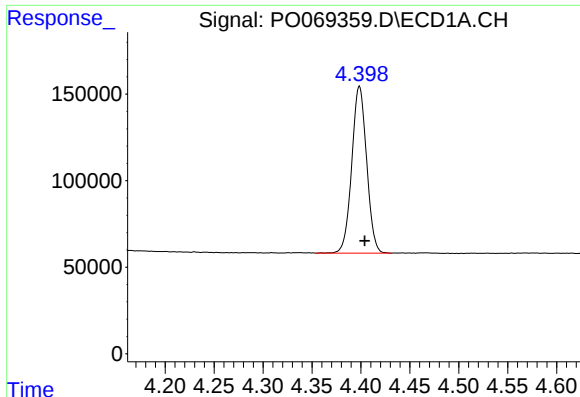

#1 Tetrachloro-m-xylene


R.T.: 4.399 min
Delta R.T.: -0.005 min
Response: 1020398
Conc: 34.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-4-S

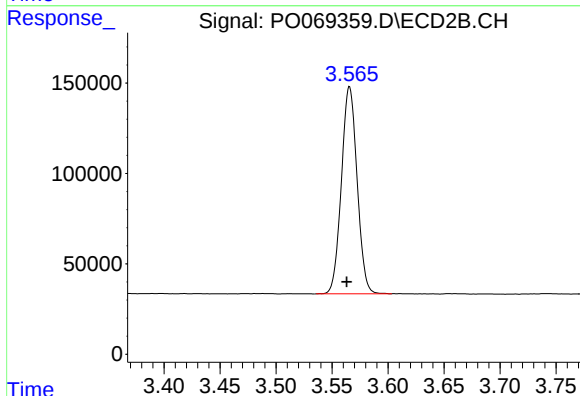


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.003 min
Response: 1117497
Conc: 29.03 ng/ml

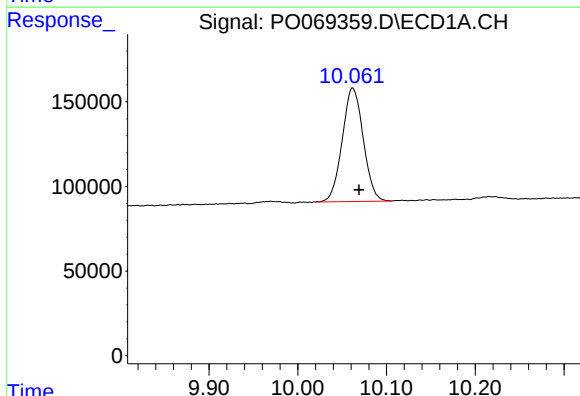

#2 Decachlorobiphenyl

R.T.: 10.062 min
Delta R.T.: -0.007 min
Response: 1105139
Conc: 23.27 ng/ml

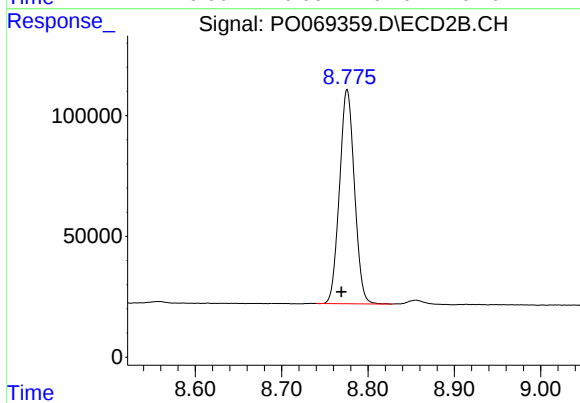

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.007 min
Response: 1066165
Conc: 19.59 ng/ml