

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070225\
 Data File : P0111992.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 19:31
 Operator : YP/AJ
 Sample : Q2481-02 50X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CC0627-CLOXPL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:43:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.673	3.722f	236982	6039652	0.041m	1.075m#
2) SA Decachlor...	8.703	8.616	931968	-17022	0.178	N.D. #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO070225\
Data File : PO111992.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 19:31
Operator : YP/AJ
Sample : Q2481-02 50X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CC0627-CLOXPL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:43:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

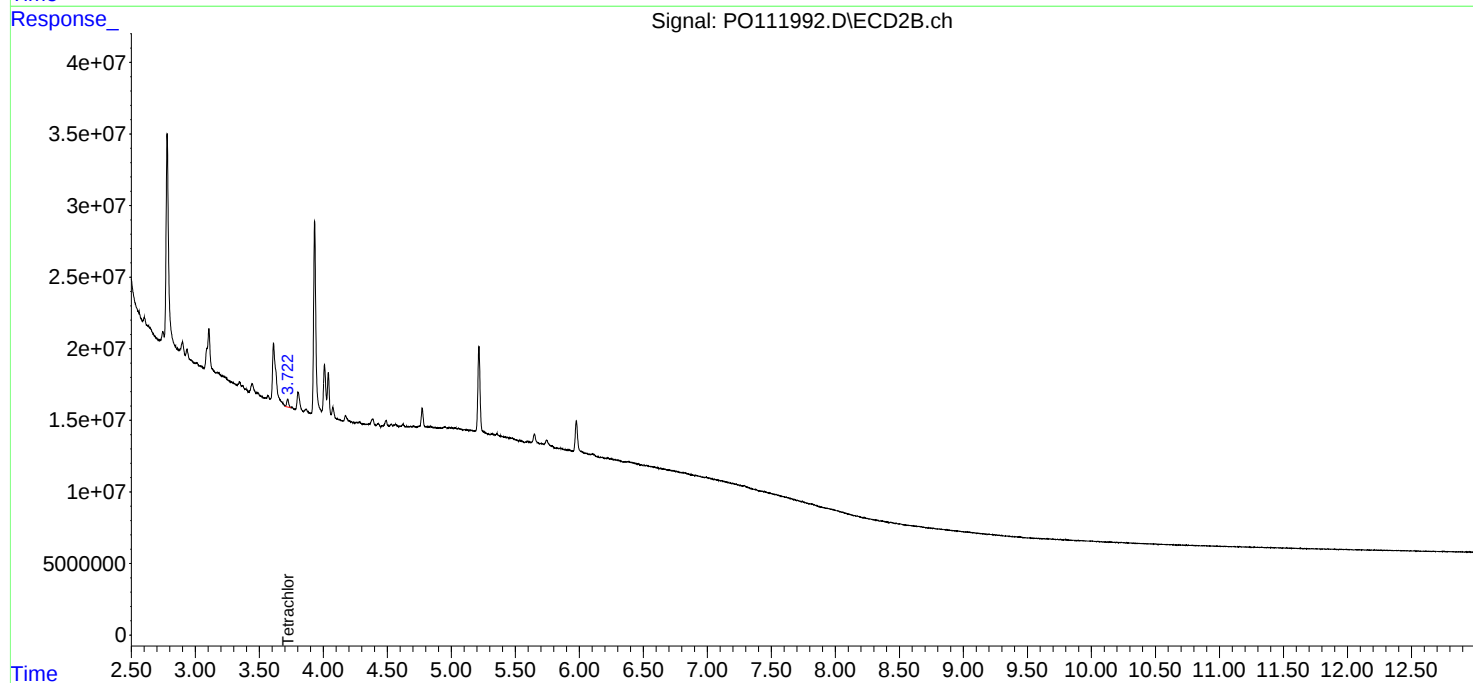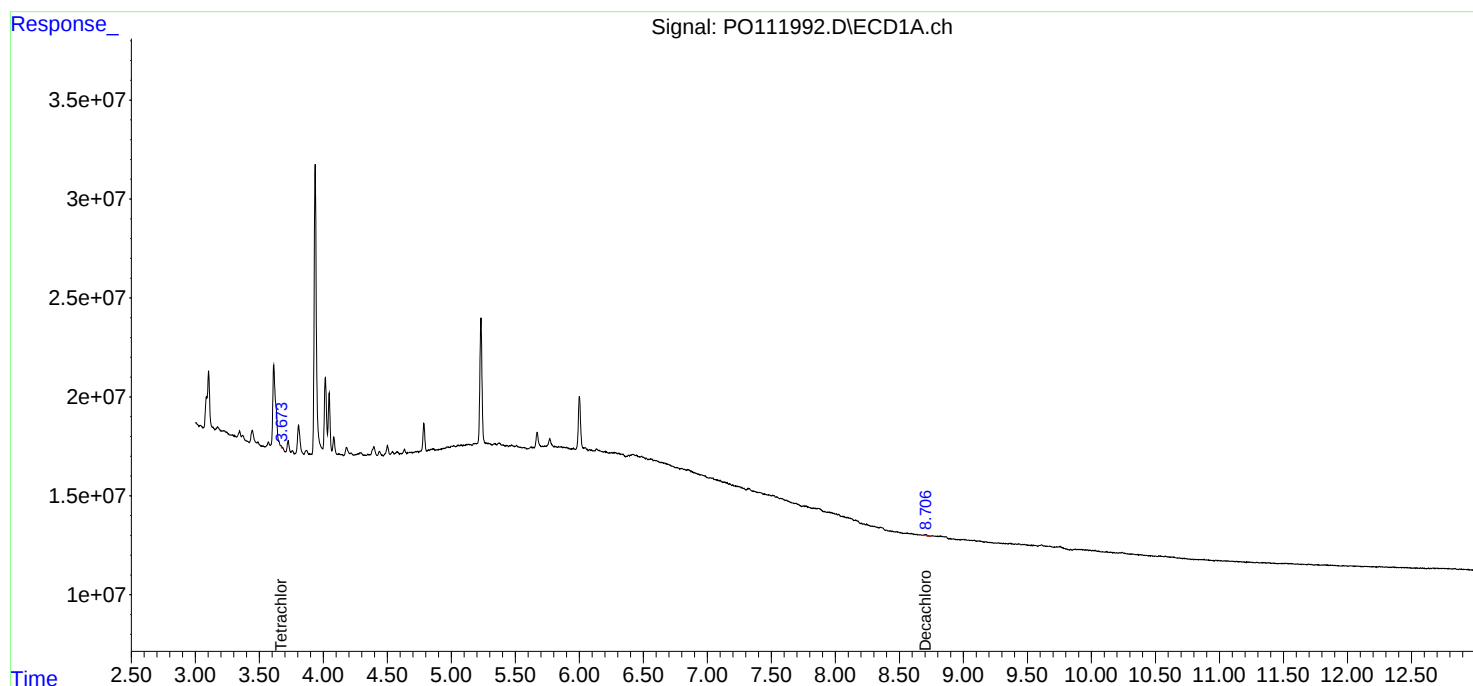

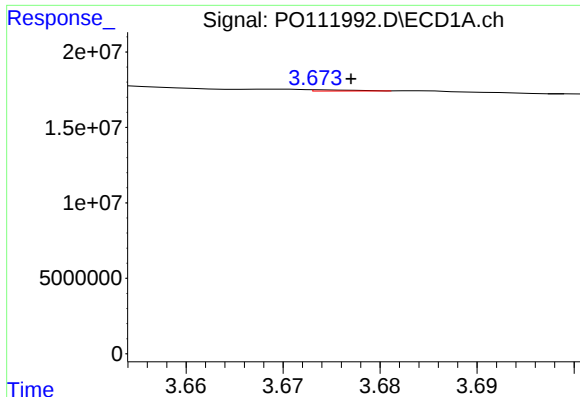


#1 Tetrachloro-m-xylene

R.T.: 3.673 min
Delta R.T.: -0.004 min
Response: 236982
Conc: 0.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC0627-CLOXPL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

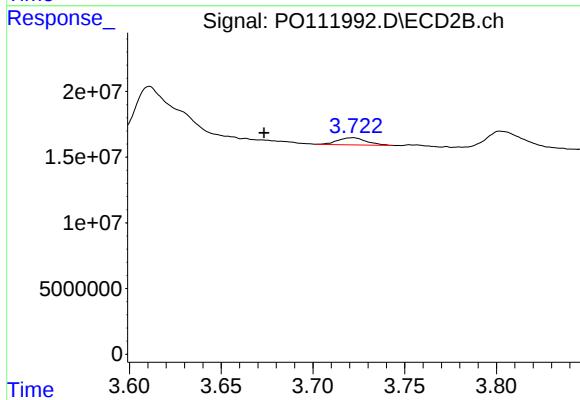


#1 Tetrachloro-m-xylene

R.T.: 3.722 min
Delta R.T.: 0.049 min
Response: 6039652
Conc: 1.08 ng/ml m

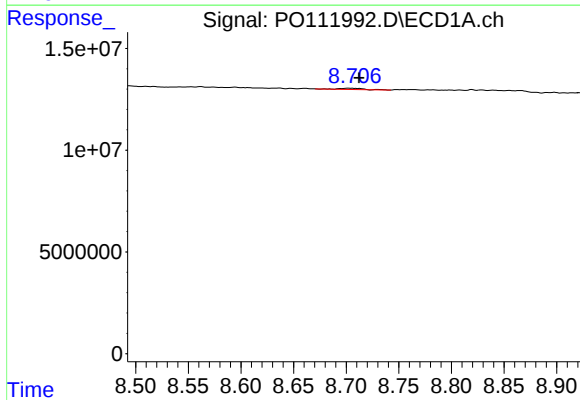

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: -0.010 min
Response: 931968
Conc: 0.18 ng/ml

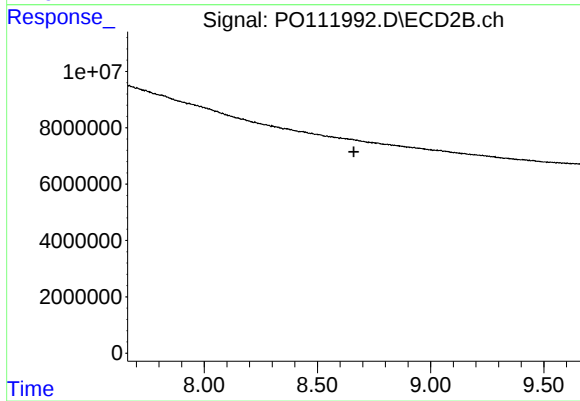

#2 Decachlorobiphenyl

R.T.: 8.616 min
Delta R.T.: -0.045 min
Response: -17022
Conc: N.D.