

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070225\
 Data File : P0111993.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Jul 2025 19:48
 Operator : YP/AJ
 Sample : Q2481-03 50X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CC0625-OXBL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/03/2025
 Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 03 01:43:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.684	3309053	3200621	0.575m	0.570m
2) SA Decachlor...	8.709	8.661	763530	407965	0.145	0.229 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070225\
Data File : PO111993.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Jul 2025 19:48
Operator : YP/AJ
Sample : Q2481-03 50X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CC0625-OXBL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/03/2025
Supervised By :mohammad ahmed 07/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 03 01:43:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

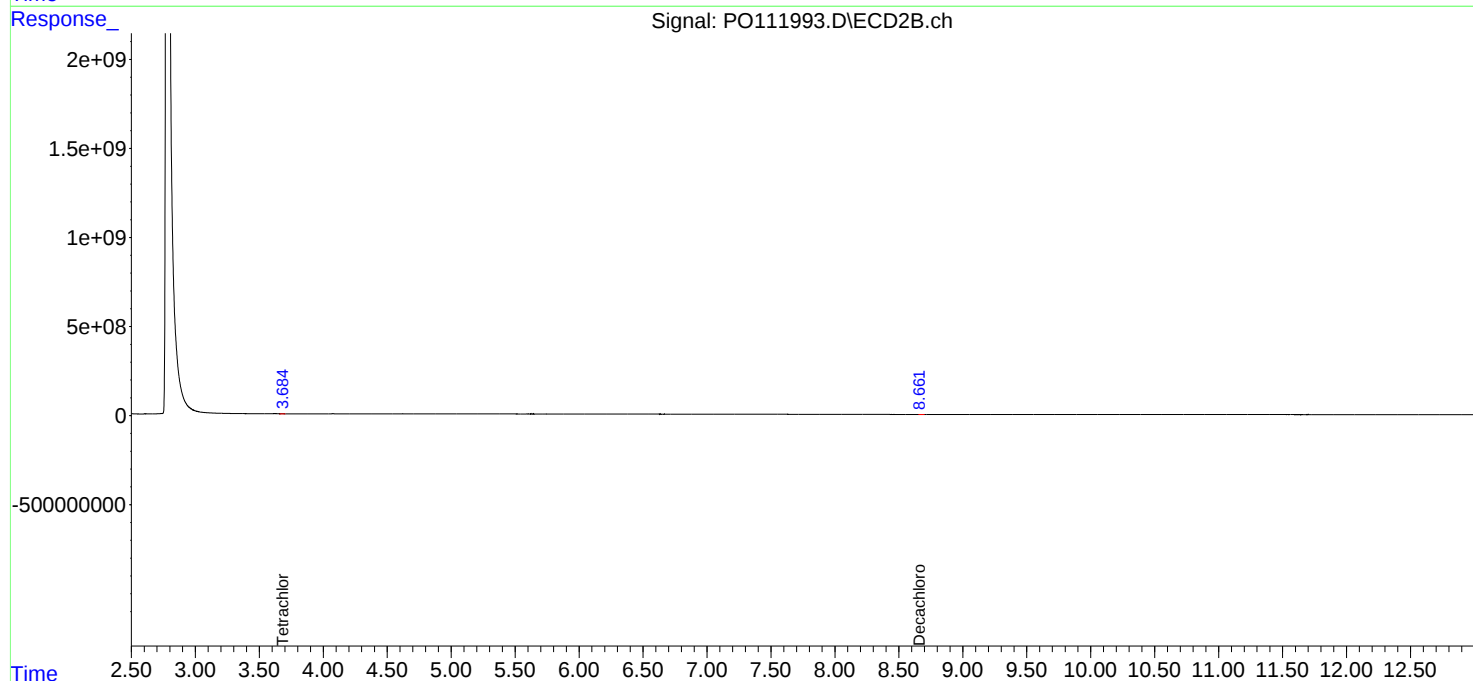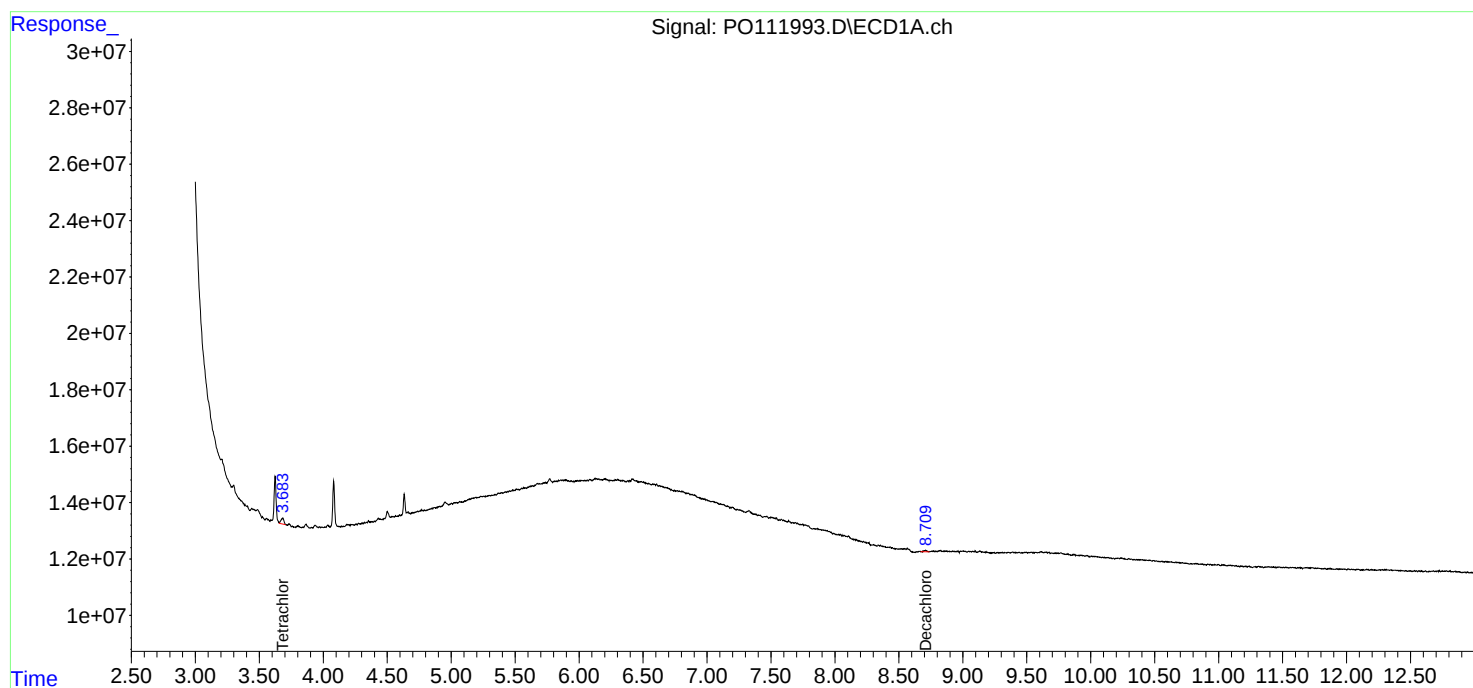

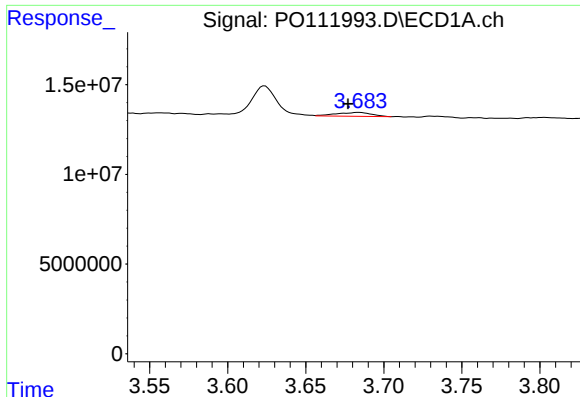

#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.006 min
Response: 3309053
Conc: 0.57 ng/ml

Instrument :

ECD_O

ClientSampleId :


CC0625-OXBL

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 07/03/2025

Supervised By :mohammad ahmed 07/04/2025

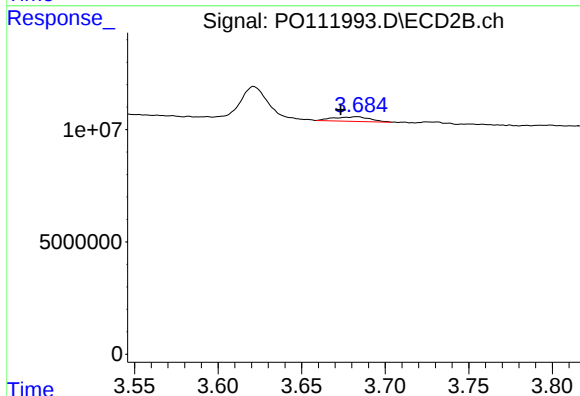


#1 Tetrachloro-m-xylene

R.T.: 3.684 min
Delta R.T.: 0.011 min
Response: 3200621
Conc: 0.57 ng/ml m

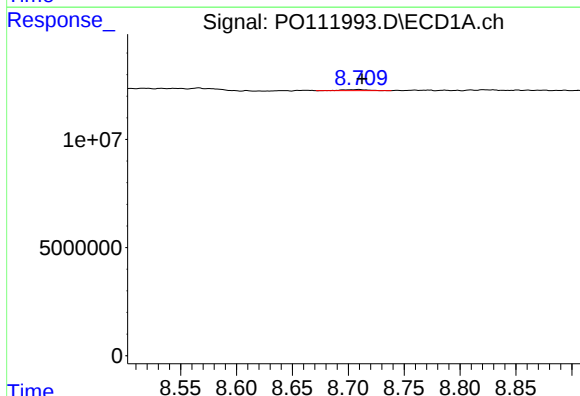

#2 Decachlorobiphenyl

R.T.: 8.709 min
Delta R.T.: -0.003 min
Response: 763530
Conc: 0.15 ng/ml

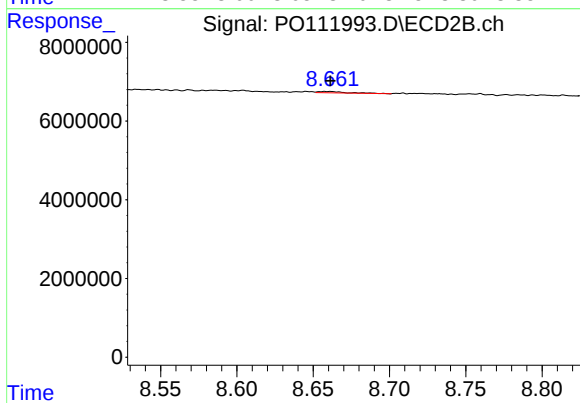

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: 0.000 min
Response: 407965
Conc: 0.23 ng/ml