

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070325\
 Data File : P0112010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Jul 2025 11:39
 Operator : YP/AJ
 Sample : Q2481-02 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 CC0627-CLOXPL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/07/2025
 Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 04 05:45:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.664	3.662	10311998	8248830	1.790m	1.468m
2) SA Decachlor...	8.705	8.651	5191298	1869346	0.989m	1.052m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070325\
Data File : PO112010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Jul 2025 11:39
Operator : YP/AJ
Sample : Q2481-02 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CC0627-CLOXPL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 04 05:45:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

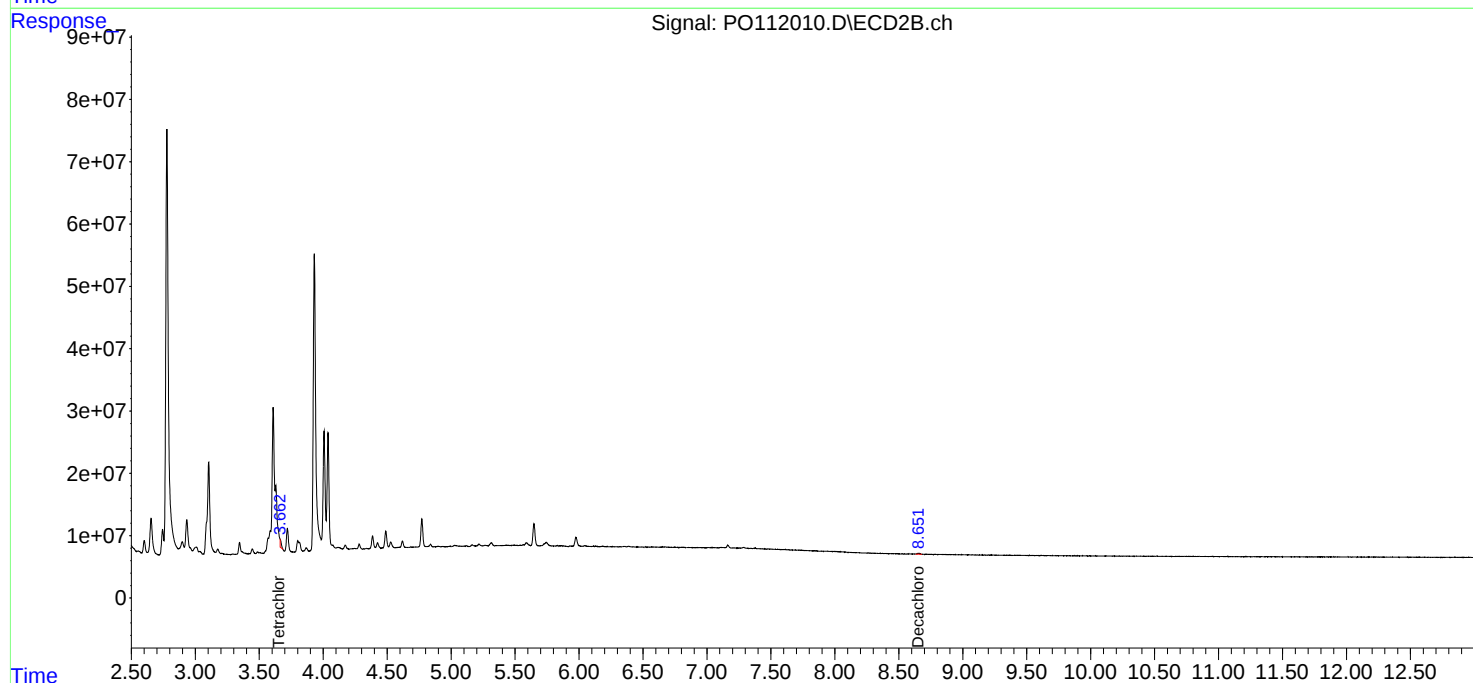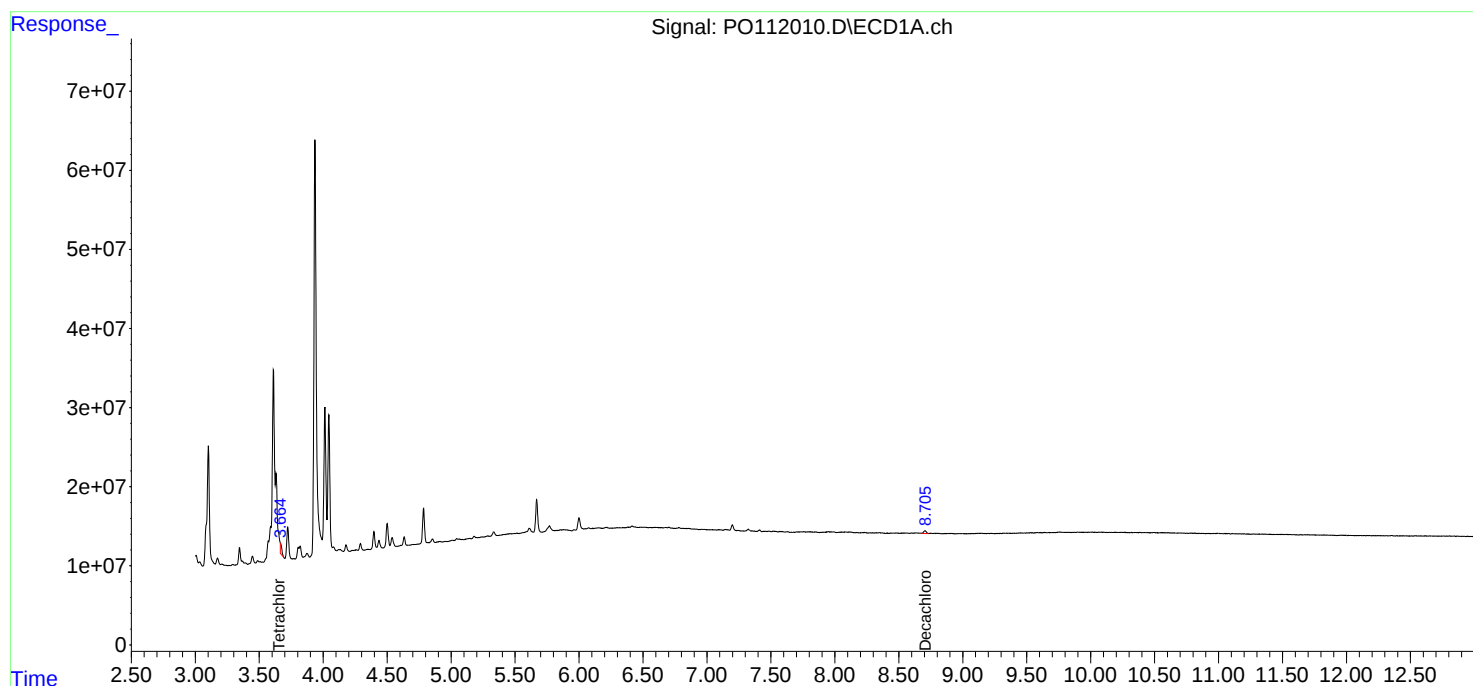

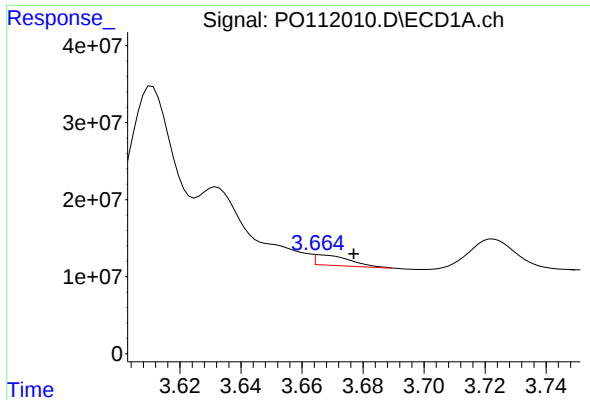


#1 Tetrachloro-m-xylene

R.T.: 3.664 min
Delta R.T.: -0.013 min
Response: 10311998
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
CC0627-CLOXPL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/07/2025
Supervised By :mohammad ahmed 07/08/2025

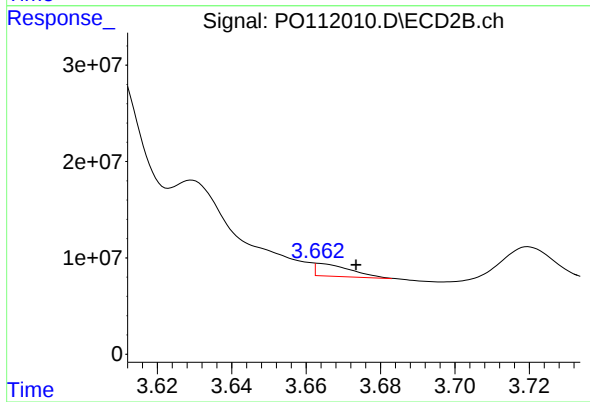


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: -0.011 min
Response: 8248830
Conc: 1.47 ng/ml m

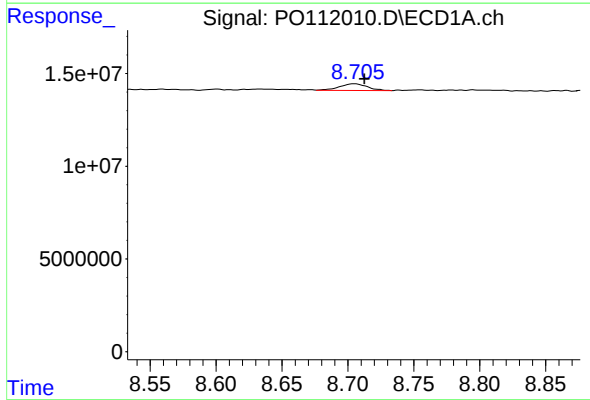

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.007 min
Response: 5191298
Conc: 0.99 ng/ml m

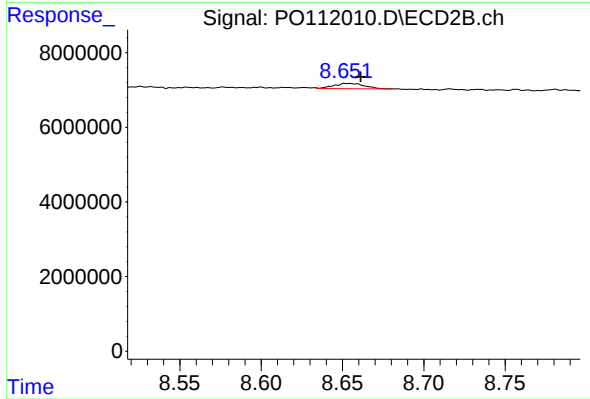

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: -0.011 min
Response: 1869346
Conc: 1.05 ng/ml m