

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
 Data File : P0069417.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2020 22:29
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 07:12:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.395	3.563	682629	724061	23.075	18.812
2)	SA Decachlor...	10.055	8.773	1193060	1166687	25.119	21.432
Target Compounds							
5)	L1 AR-1016-3	5.815	0.000	5177152	0	4628.585	N.D. #
18)	L4 AR-1242-3	5.815	0.000	5177152	0	6002.144	N.D. #
20)	L4 AR-1242-5	6.663	0.000	6314194	0	7076.063	N.D. #
24)	L5 AR-1248-4	6.663	0.000	6314194	0	4198.354	N.D. #
25)	L5 AR-1248-5	6.663	0.000	6314194	0	4360.325	N.D. #
26)	L6 AR-1254-1	6.663	0.000	6314194	0	4299.044	N.D. #
28)	L6 AR-1254-3	7.180	0.000	1513903	0	587.493	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070620\
Data File : PO069417.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2020 22:29
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 07:12:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

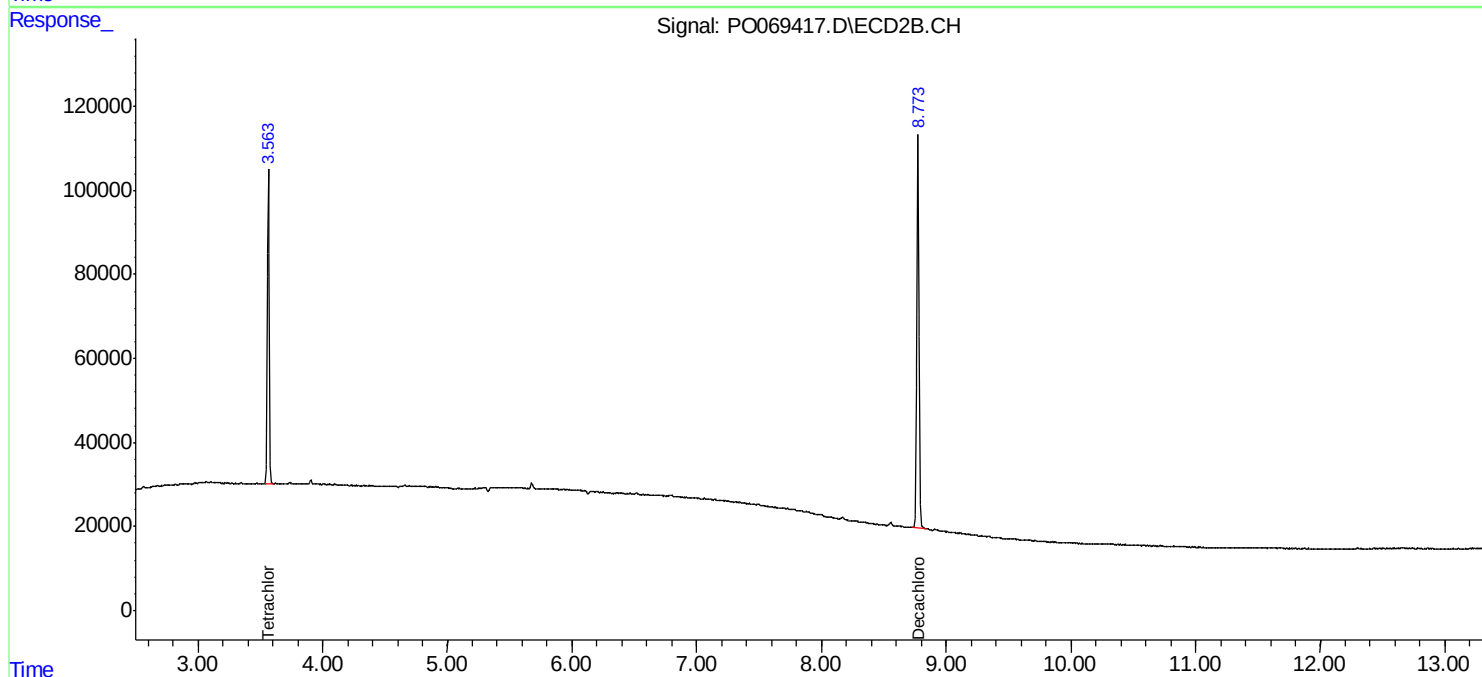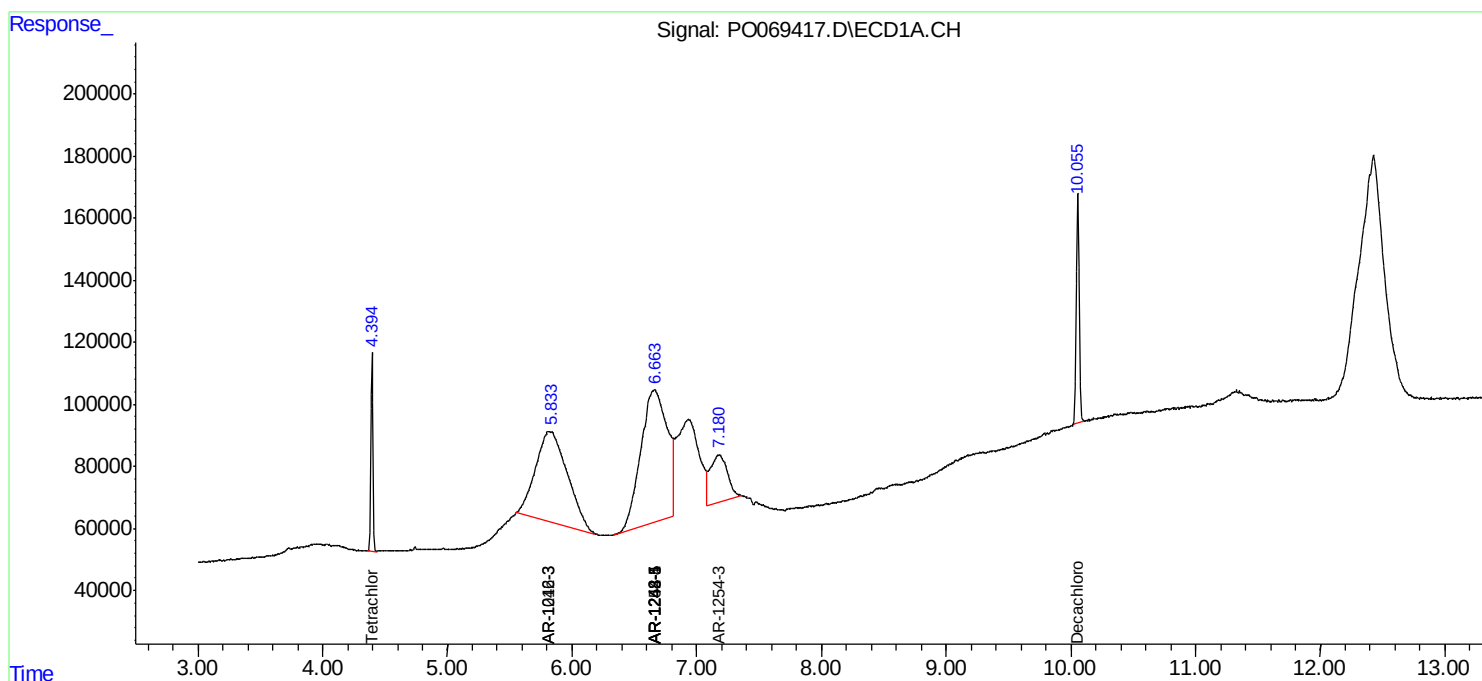


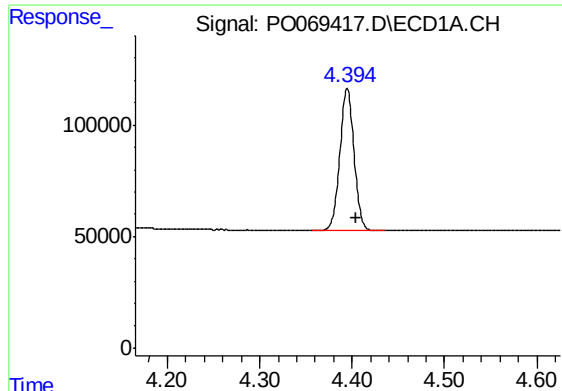

#1 Tetrachloro-m-xylene


R.T.: 4.395 min
Delta R.T.: -0.009 min
Response: 682629
Conc: 23.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

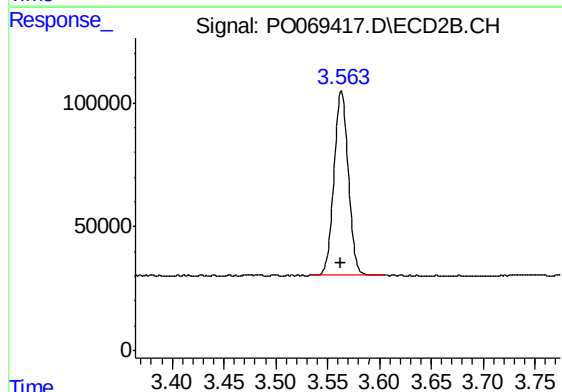


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 724061
Conc: 18.81 ng/ml

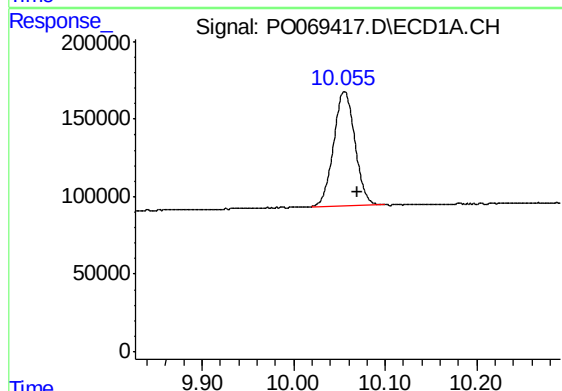


#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: -0.014 min
Response: 1193060
Conc: 25.12 ng/ml

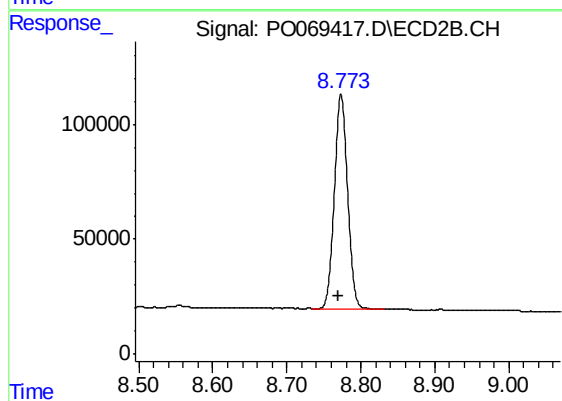

#2 Decachlorobiphenyl


R.T.: 8.773 min
Delta R.T.: 0.004 min
Response: 1166687
Conc: 21.43 ng/ml

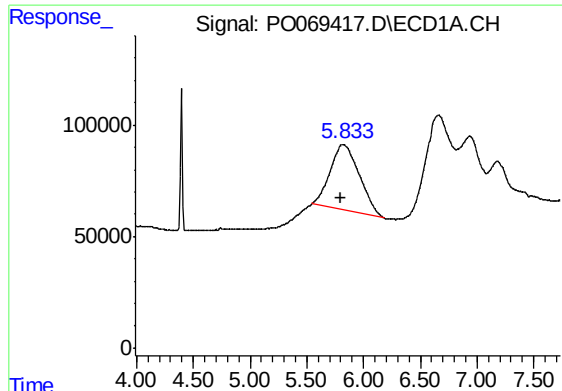

#5 AR-1016-3


R.T.: 5.815 min
Delta R.T.: 0.017 min
Response: 5177152
Conc: 4628.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

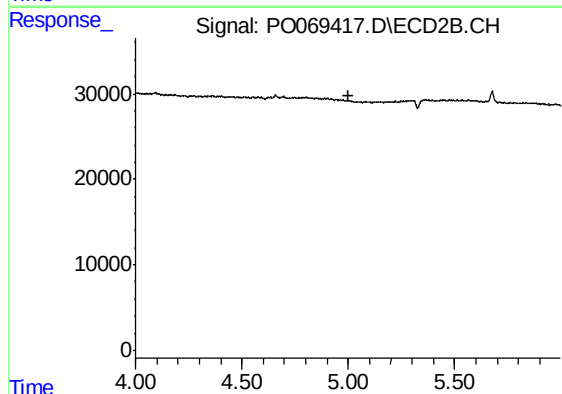


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.999 min
Response: 0
Conc: N.D.

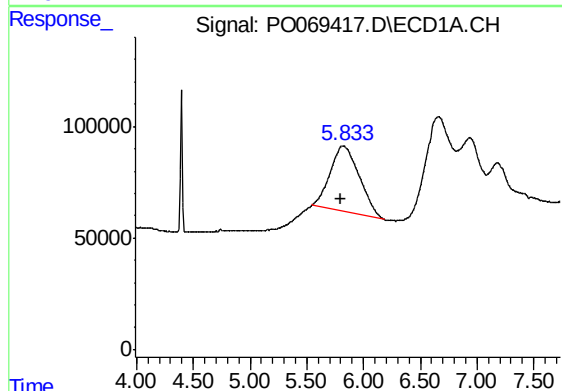


#18 AR-1242-3

R.T.: 5.815 min
Delta R.T.: 0.016 min
Response: 5177152
Conc: 6002.14 ng/ml

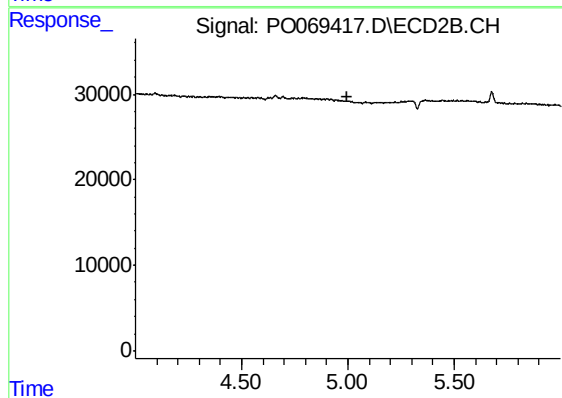

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 5.000 min
Response: 0
Conc: N.D.

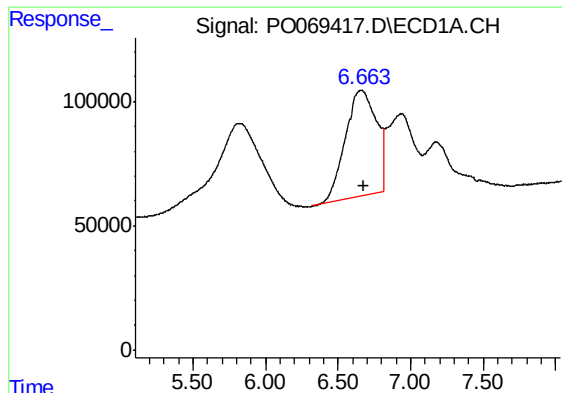

#20 AR-1242-5


R.T.: 6.663 min
Delta R.T.: -0.016 min
Response: 6314194
Conc: 7076.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

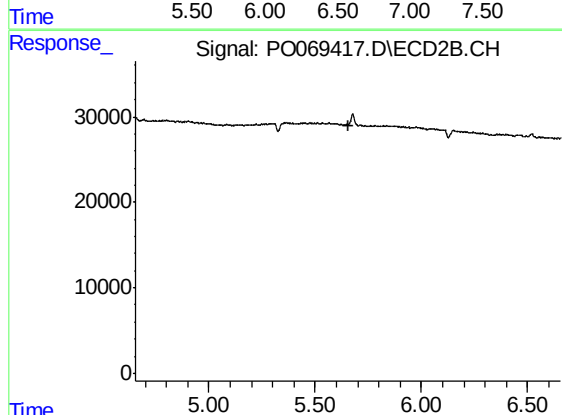


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.655 min
Response: 0
Conc: N.D.

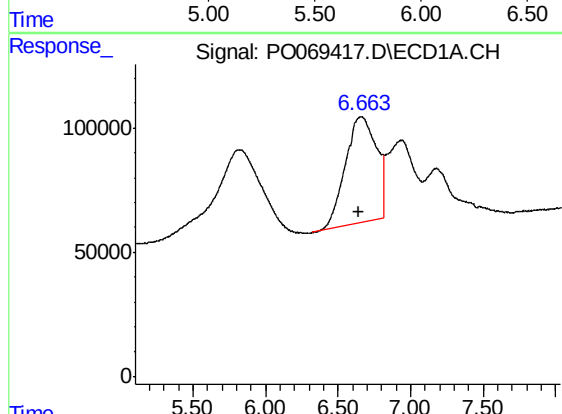


#24 AR-1248-4

R.T.: 6.663 min
Delta R.T.: 0.022 min
Response: 6314194
Conc: 4198.35 ng/ml

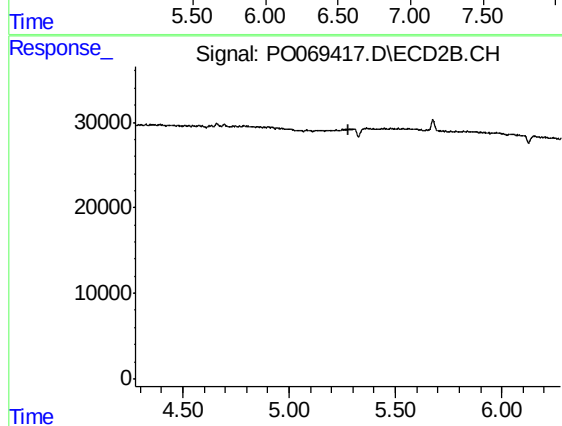

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

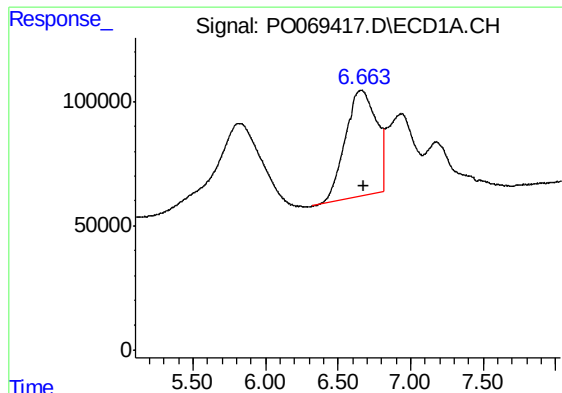

#25 AR-1248-5


R.T.: 6.663 min
Delta R.T.: -0.015 min
Response: 6314194
Conc: 4360.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

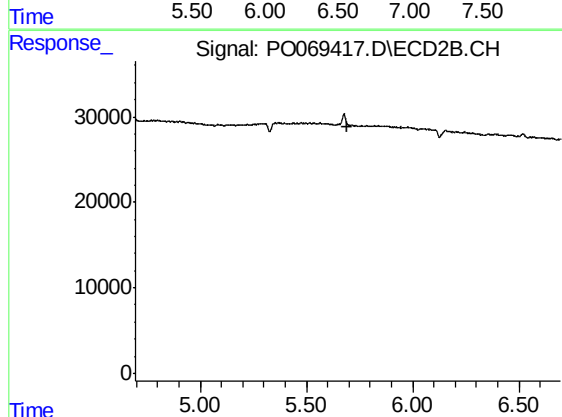


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.695 min
Response: 0
Conc: N.D.

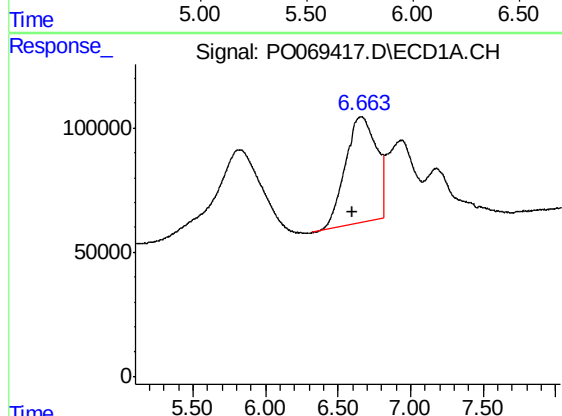


#26 AR-1254-1

R.T.: 6.663 min
Delta R.T.: 0.059 min
Response: 6314194
Conc: 4299.04 ng/ml

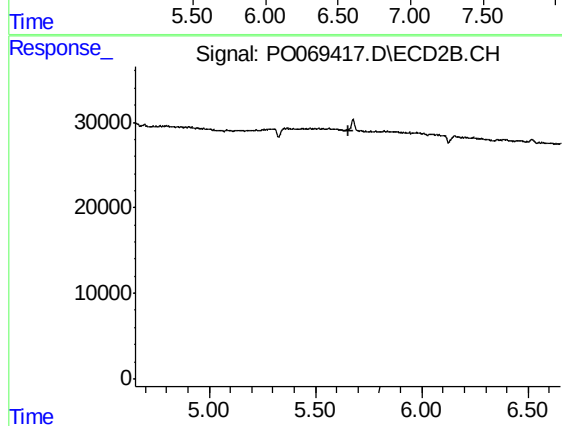

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 5.653 min
Response: 0
Conc: N.D.

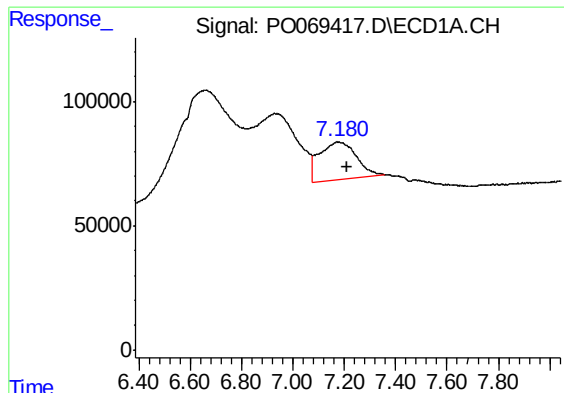

#28 AR-1254-3

R.T.: 7.180 min
Delta R.T.: -0.029 min
Response: 1513903
Conc: 587.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

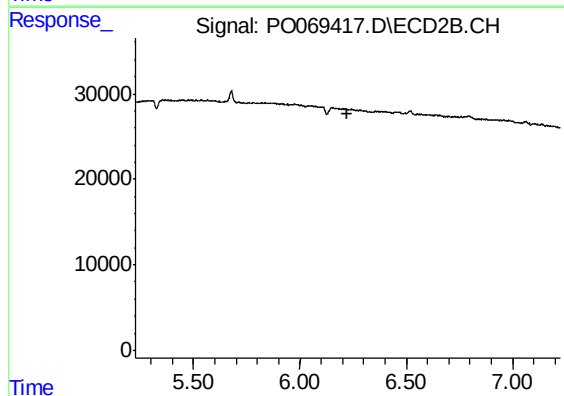

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.226 min
Response: 0
Conc: N.D.