

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
 Data File : P0069395.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2020 11:07
 Operator : DD\AJ
 Sample : L3175-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PRESS-SAMPLE

Manual Integrations
 APPROVED

Ankita
 7/7/2020 1:12:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 14:08:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.567	757451	1203392	25.604	31.266
2) SA Decachlor...	10.065	8.785	2305427	4407594	48.539m	80.969m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
Data File : P0069395.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2020 11:07
Operator : DD\AJ
Sample : L3175-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PRESS-SAMPLE


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 14:08:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

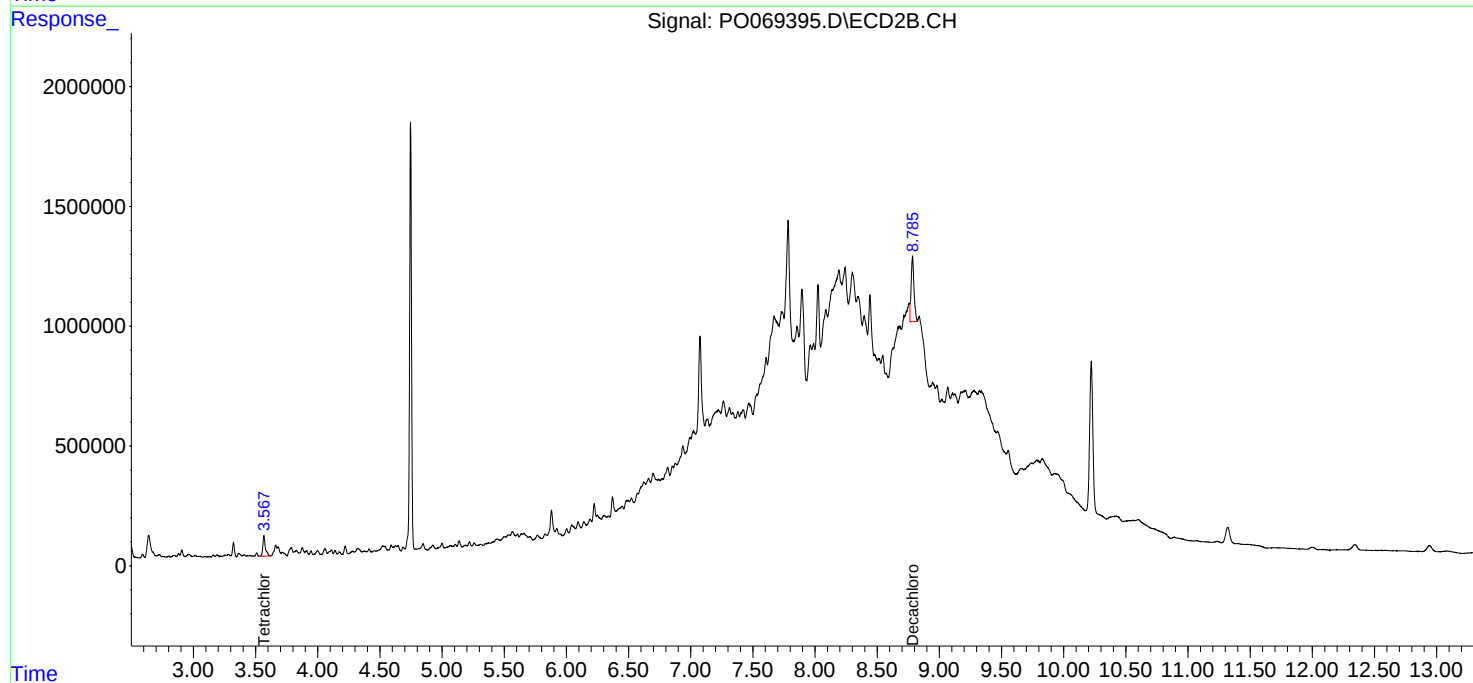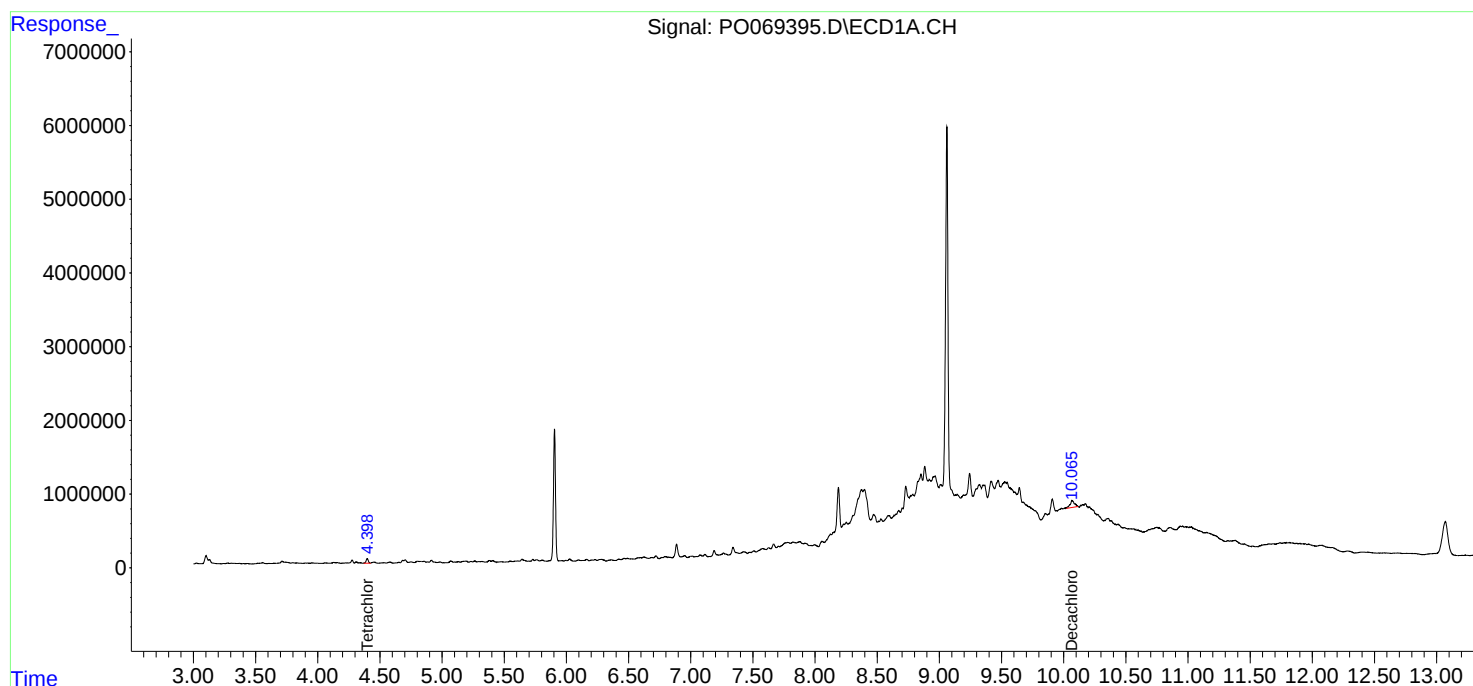

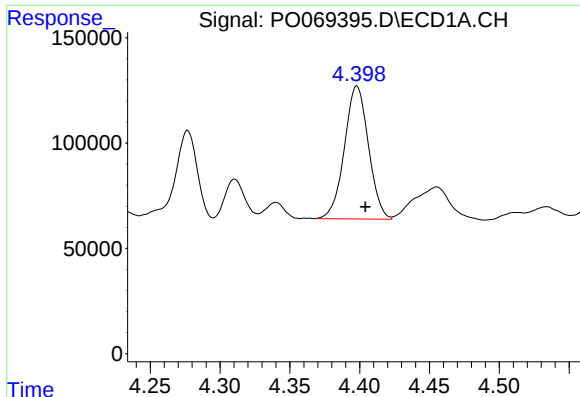


#1 Tetrachloro-m-xylene

R.T.: 4.398 min
Delta R.T.: -0.006 min
Response: 757451
Conc: 25.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
PRESS-SAMPLE


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:39 PM

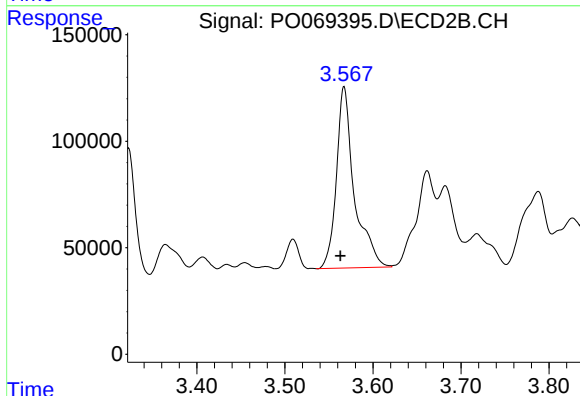


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.004 min
Response: 1203392
Conc: 31.27 ng/ml

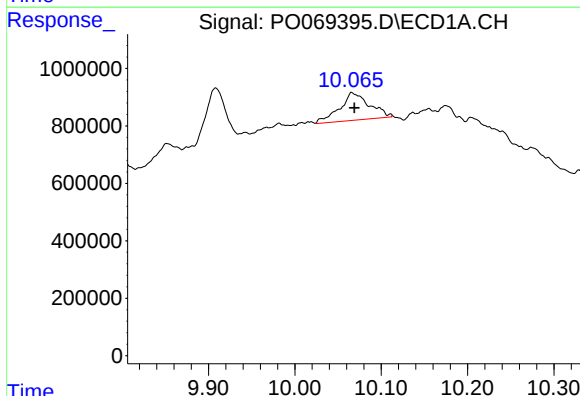

#2 Decachlorobiphenyl

R.T.: 10.065 min
Delta R.T.: -0.004 min
Response: 2305427
Conc: 48.54 ng/ml m

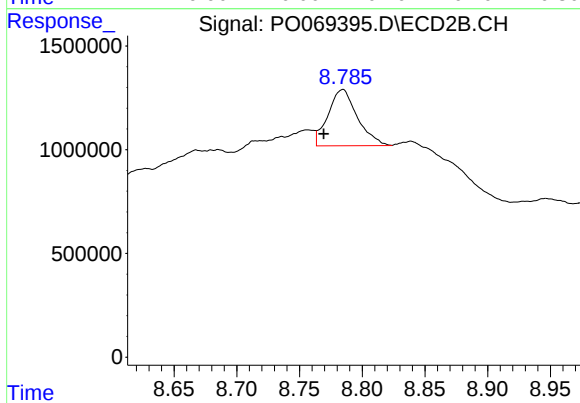

#2 Decachlorobiphenyl

R.T.: 8.785 min
Delta R.T.: 0.015 min
Response: 4407594
Conc: 80.97 ng/ml m