

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
 Data File : P0069397.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2020 12:33
 Operator : DD\AJ
 Sample : L3174-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 19569

Manual Integrations
 APPROVED

Ankita
 7/7/2020 1:12:43 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 06 14:09:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.574	1129325	1129973	38.175	29.358
2) SA Decachlor...	10.096	8.815	1048909	891616	22.084	16.379m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
Data File : P0069397.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2020 12:33
Operator : DD\AJ
Sample : L3174-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
19569


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:43 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 06 14:09:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

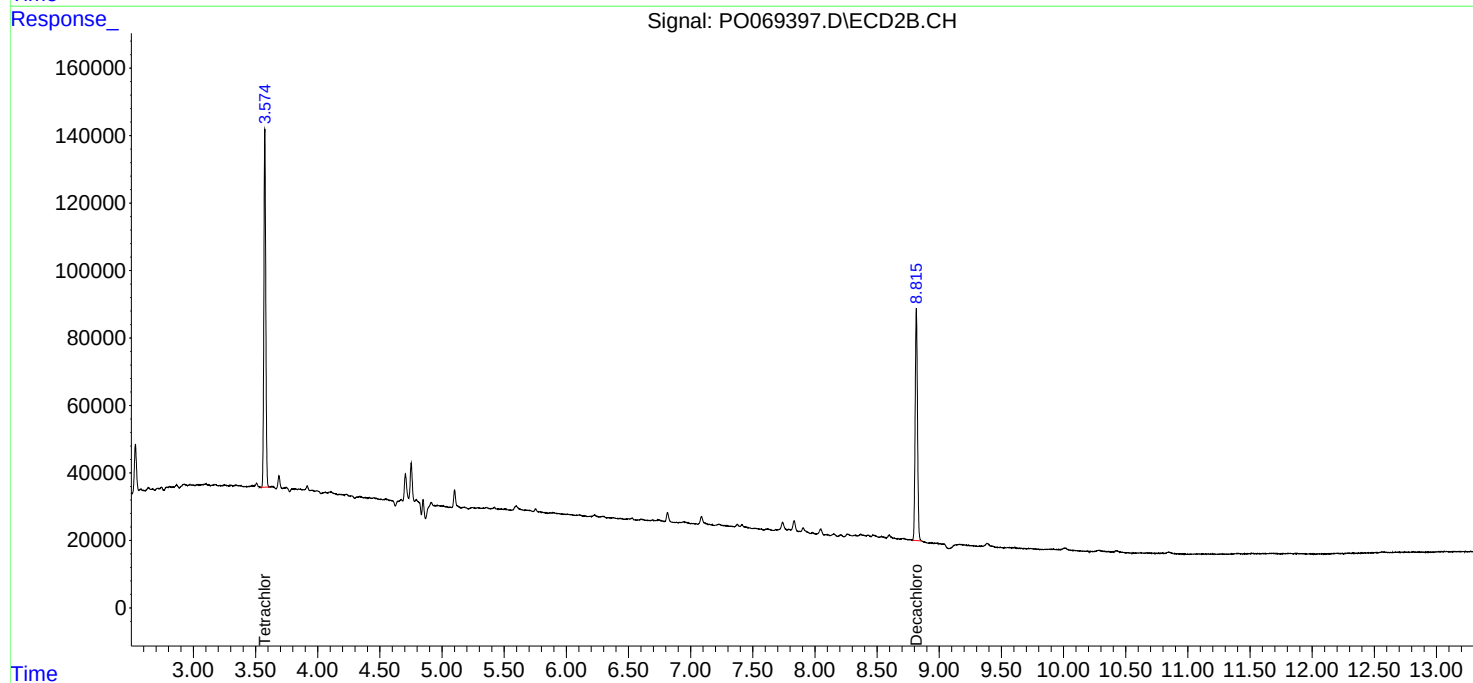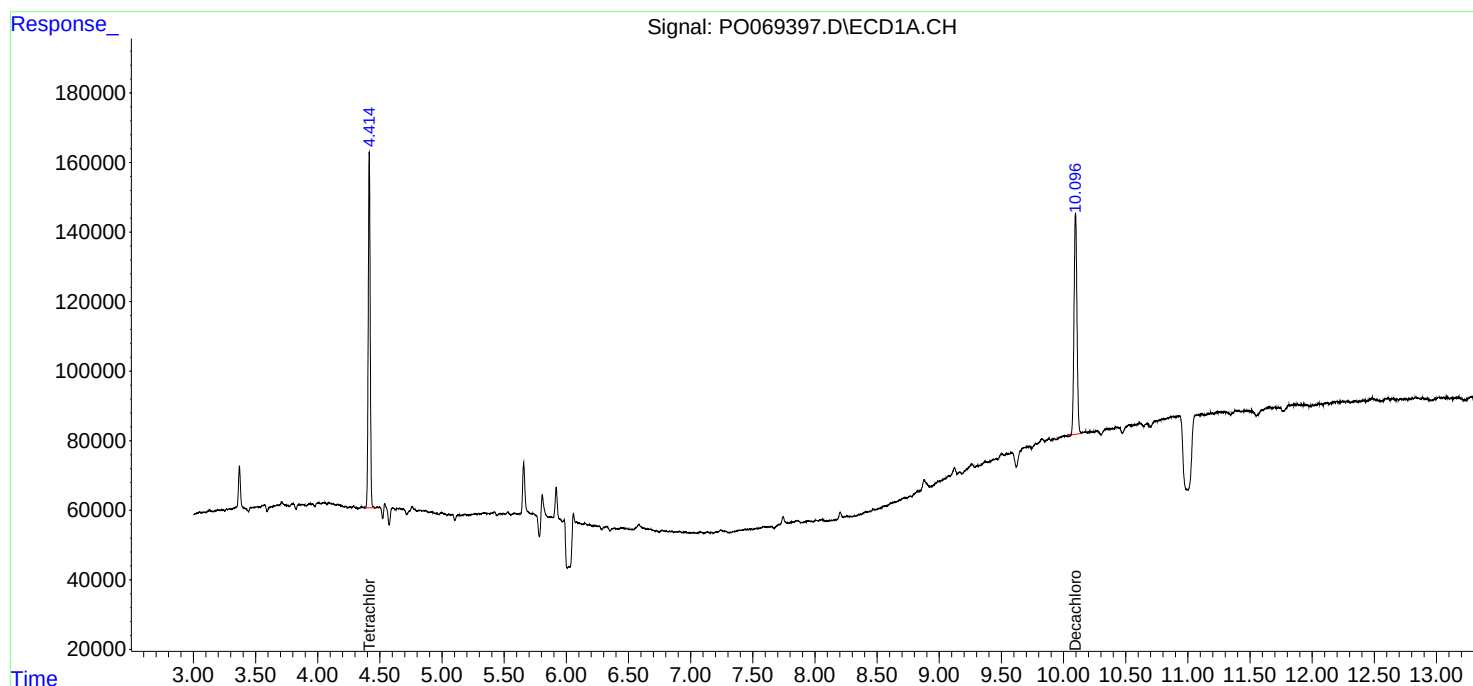

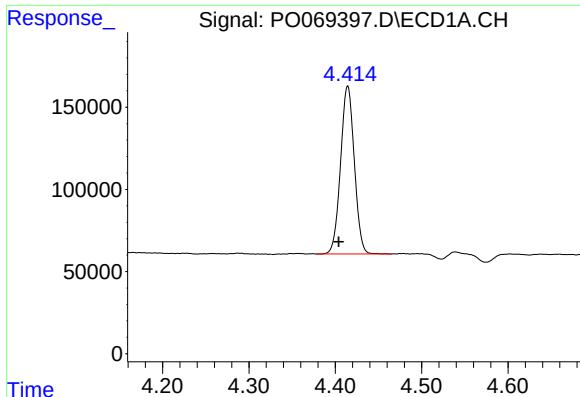


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: 0.011 min
Response: 1129325
Conc: 38.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
19569


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:43 PM

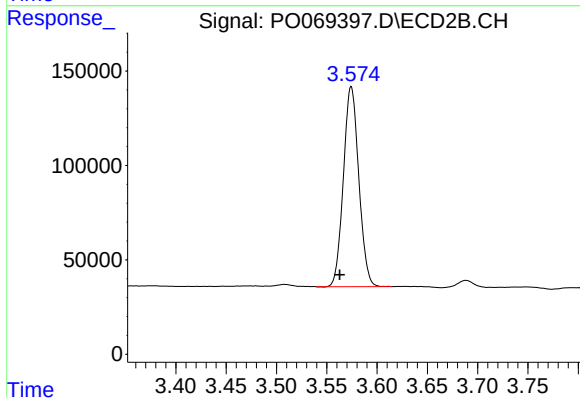


#1 Tetrachloro-m-xylene

R.T.: 3.574 min
Delta R.T.: 0.011 min
Response: 1129973
Conc: 29.36 ng/ml

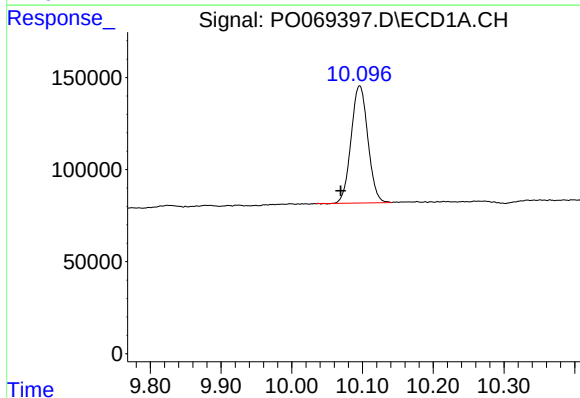

#2 Decachlorobiphenyl

R.T.: 10.096 min
Delta R.T.: 0.027 min
Response: 1048909
Conc: 22.08 ng/ml

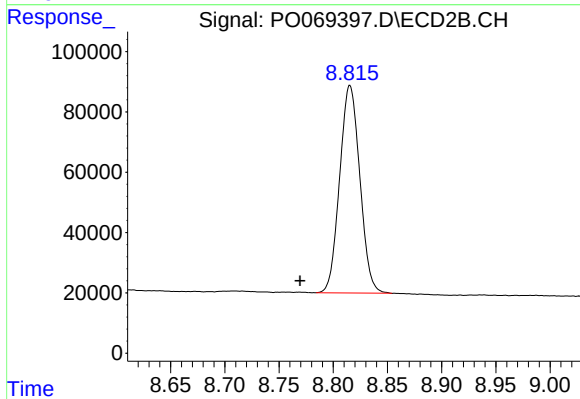

#2 Decachlorobiphenyl

R.T.: 8.815 min
Delta R.T.: 0.046 min
Response: 891616
Conc: 16.38 ng/ml m