

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
 Data File : P0069412.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2020 20:29
 Operator : DD\AJ
 Sample : L3223-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-062220-SR-08

Manual Integrations
 APPROVED

Ankita
 7/7/2020 1:12:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 07:09:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.396	3.564	177881	188116	6.013	4.887
2) SA Decachlor...	10.055	8.773	177957	230582	3.747m	4.236m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070620\
Data File : P0069412.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2020 20:29
Operator : DD\AJ
Sample : L3223-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-08


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 07:09:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

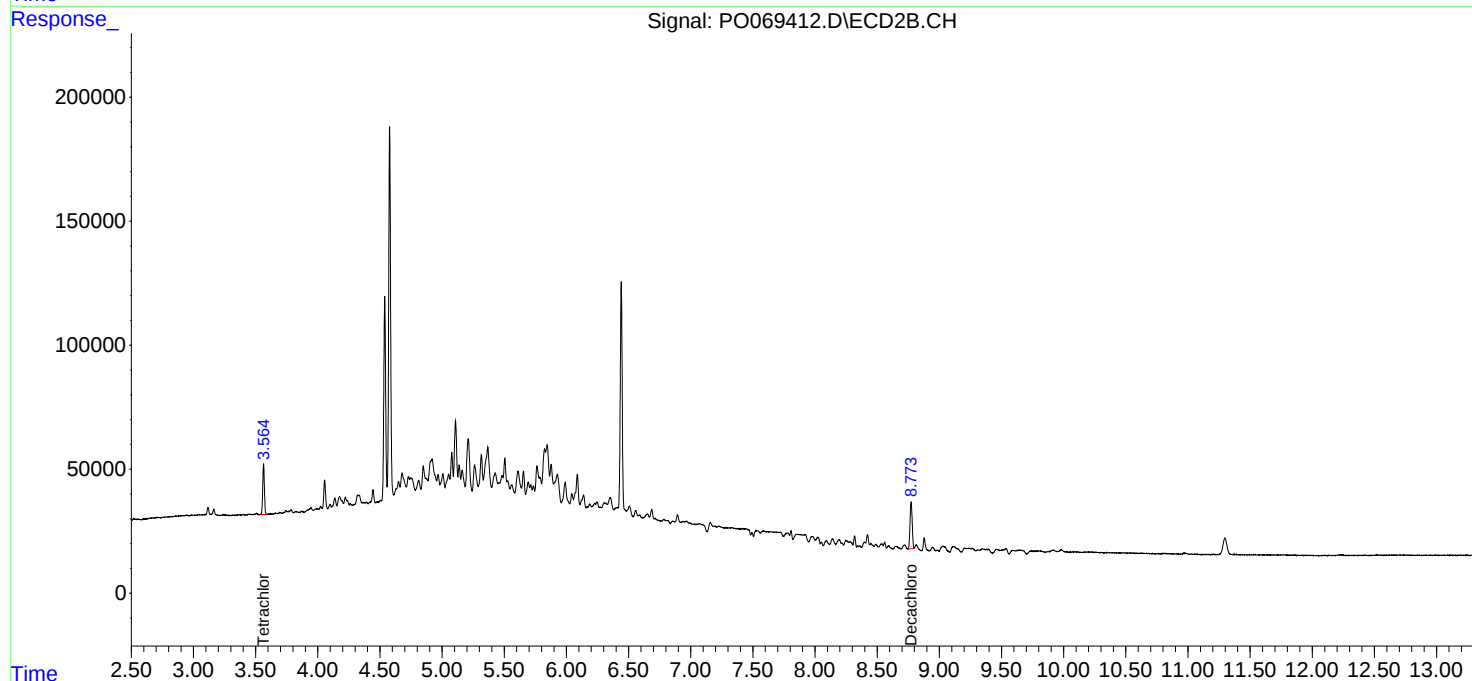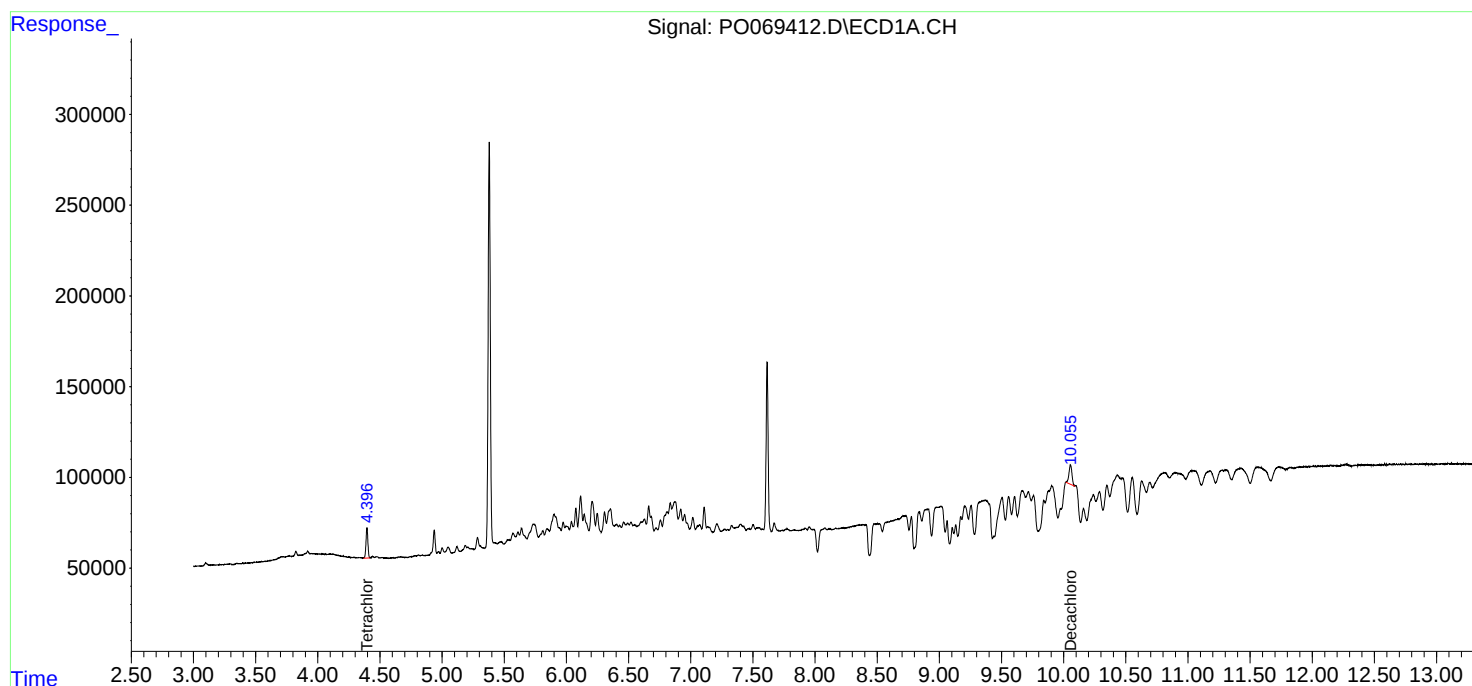

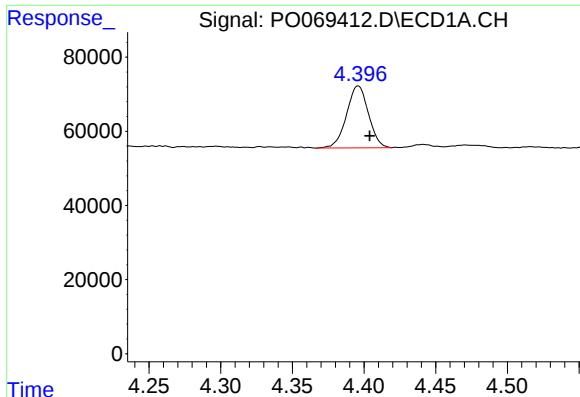


#1 Tetrachloro-m-xylene

R.T.: 4.396 min
Delta R.T.: -0.008 min
Response: 177881
Conc: 6.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-08


Manual Integrations
APPROVED

Ankita
7/7/2020 1:12:54 PM

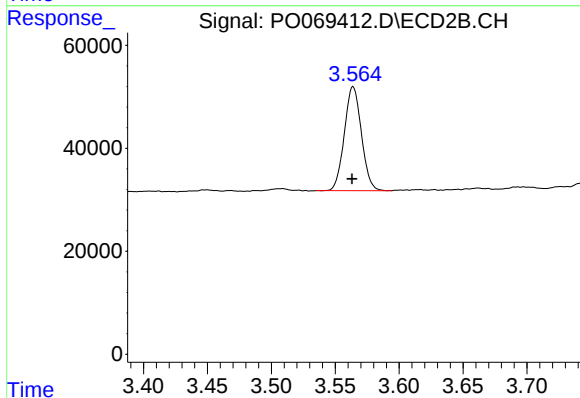


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 188116
Conc: 4.89 ng/ml

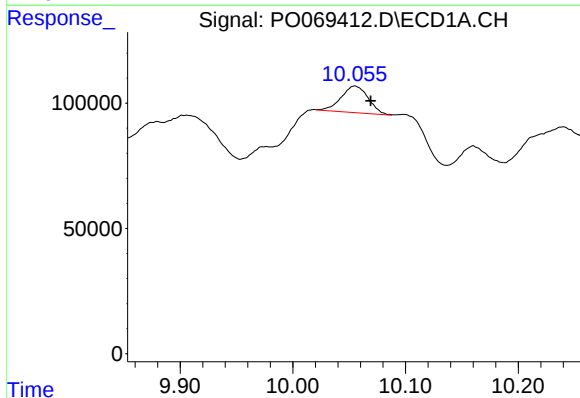

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: -0.014 min
Response: 177957
Conc: 3.75 ng/ml m

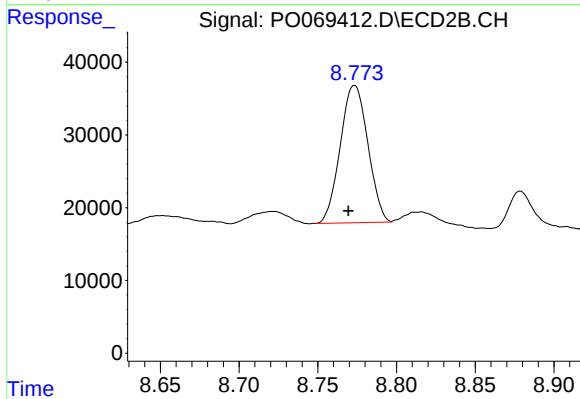

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: 0.004 min
Response: 230582
Conc: 4.24 ng/ml m