

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
 Data File : P0079328.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2021 16:46
 Operator : DD\AJ
 Sample : M2938-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 02:31:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 02 07:33:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.020	4.224	1282752	593226	22.013	20.166
2)	SA Decachlor...	11.149	9.669	825244	434503	19.540	16.610
Target Compounds							
8)	L2 AR-1221-1	5.273	0.000	123455	0	193.830	N.D. #
9)	L2 AR-1221-2	0.000	4.586	0	26373	N.D.	101.368 #
20)	L4 AR-1242-5	0.000	6.402	0	14241	N.D.	18.958 #
26)	L6 AR-1254-1	0.000	6.402	0	14241	N.D.	8.916 #
28)	L6 AR-1254-3	7.893	0.000	56929	0	16.099	N.D. #
32)	L7 AR-1260-2	8.312	0.000	77142	0	28.056	N.D. #
43)	L9 AR-1268-3	0.000	8.789	0	44754	N.D.	17.390 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079328.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 16:46
Operator : DD\AJ
Sample : M2938-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 02:31:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

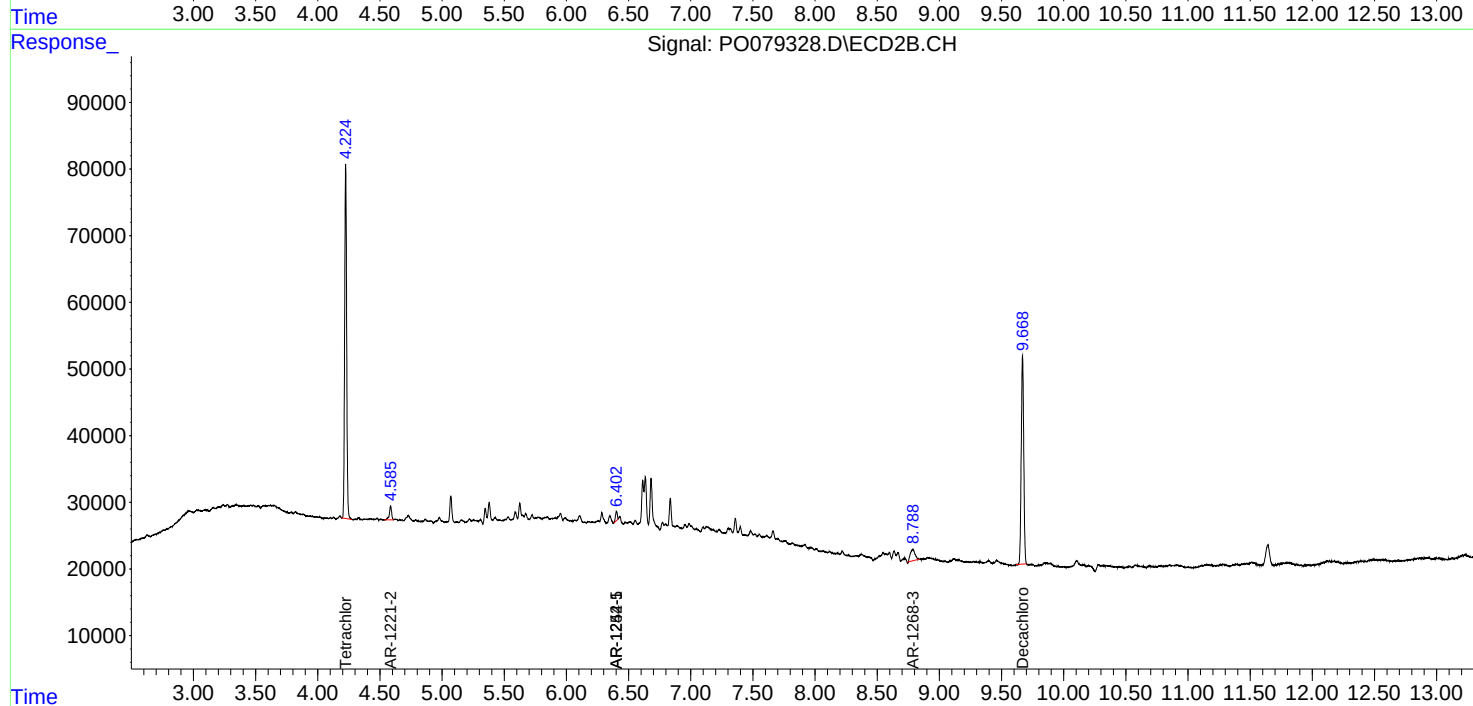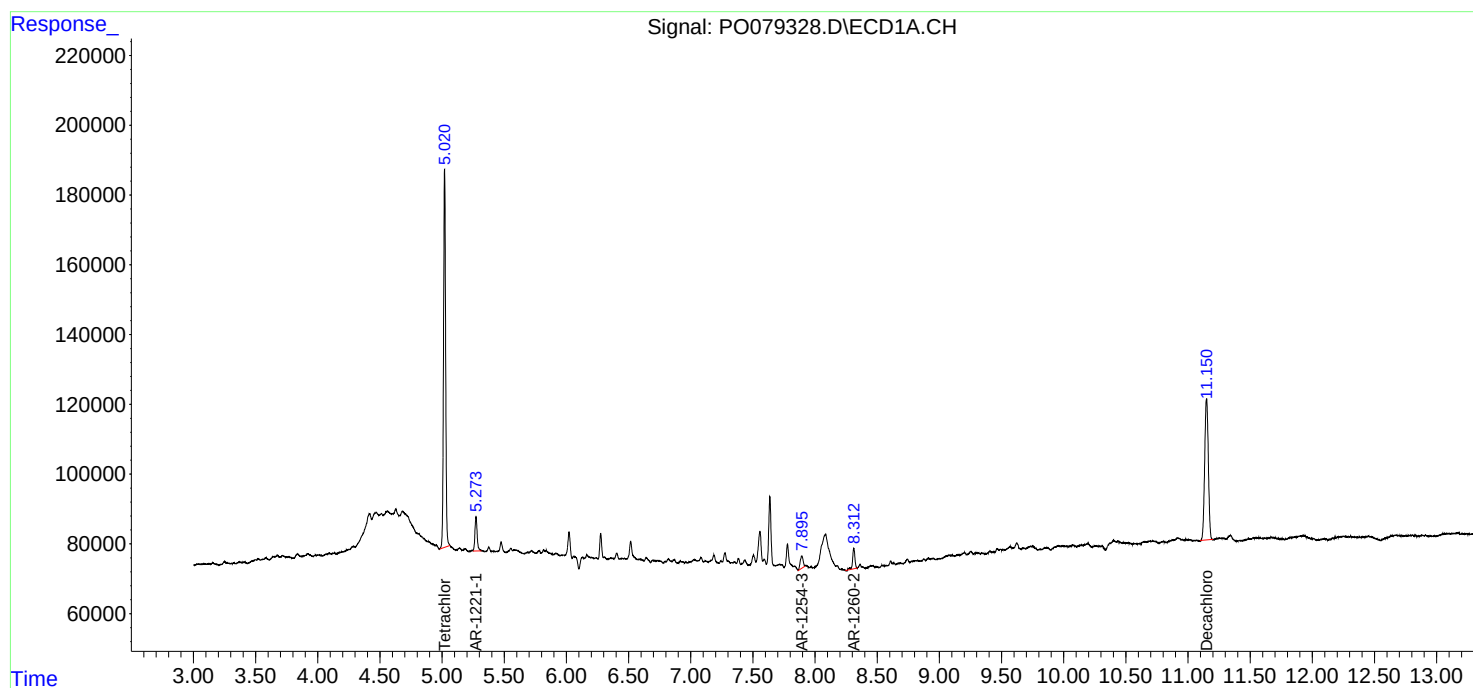


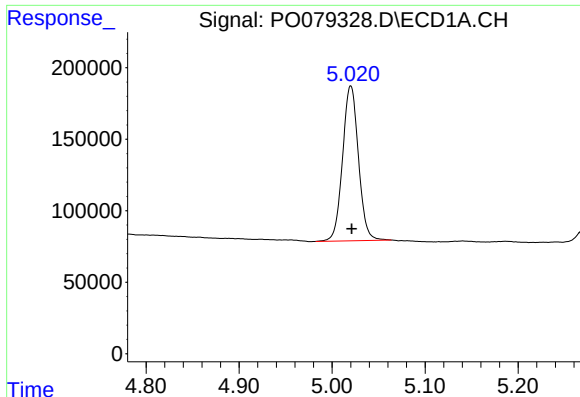

#1 Tetrachloro-m-xylene


R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 1282752
Conc: 22.01 ng/ml

Instrument :
ECD_O
ClientSampleId :

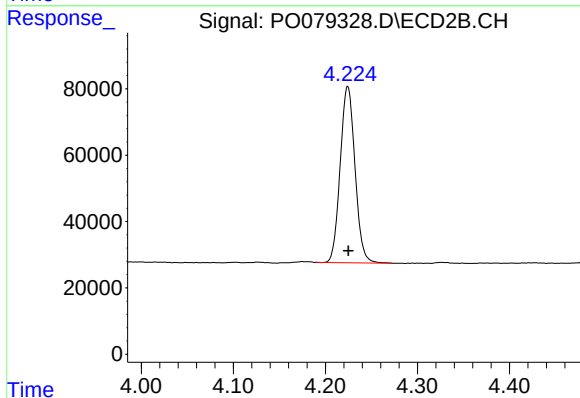


#1 Tetrachloro-m-xylene

R.T.: 4.224 min
Delta R.T.: 0.000 min
Response: 593226
Conc: 20.17 ng/ml

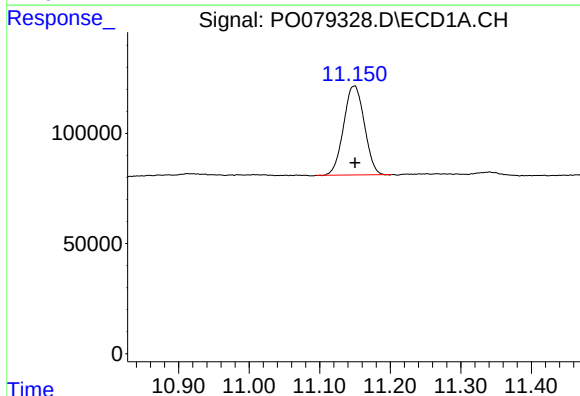


#2 Decachlorobiphenyl

R.T.: 11.149 min
Delta R.T.: 0.000 min
Response: 825244
Conc: 19.54 ng/ml

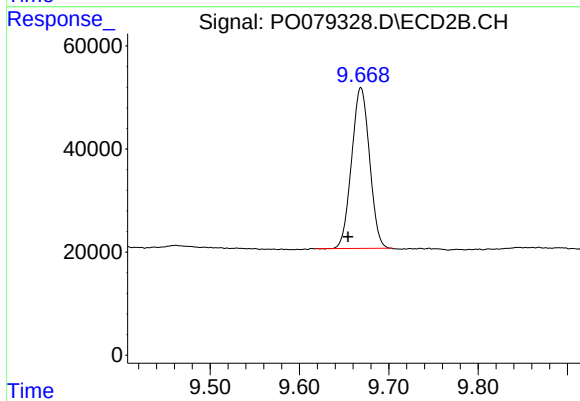

#2 Decachlorobiphenyl


R.T.: 9.669 min
Delta R.T.: 0.014 min
Response: 434503
Conc: 16.61 ng/ml

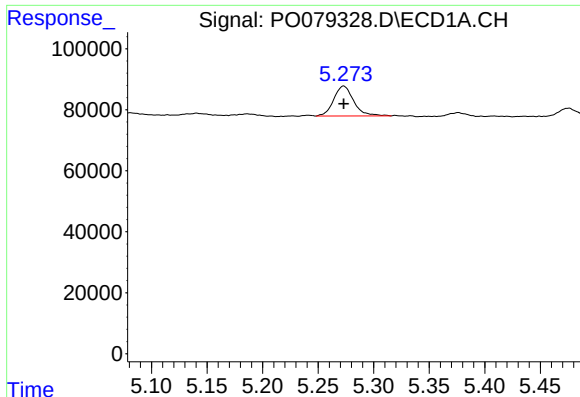

#8 AR-1221-1


R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 123455
Conc: 193.83 ng/ml

Instrument :
ECD_O
ClientSampleId :

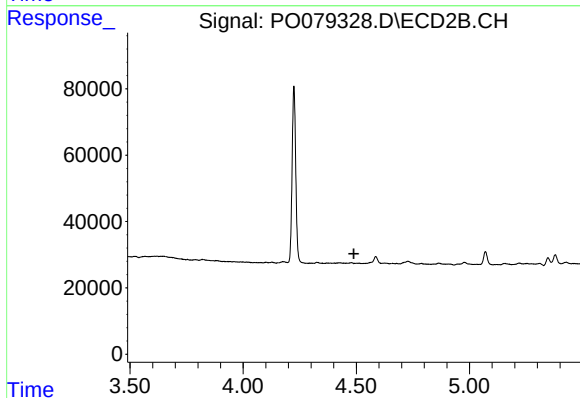


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.489 min
Response: 0
Conc: N.D.

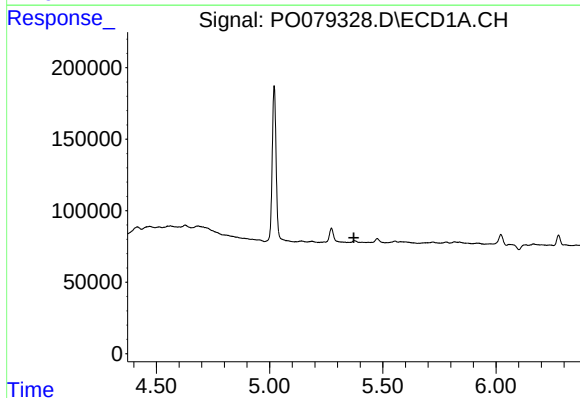


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 5.372 min
Response: 0
Conc: N.D.

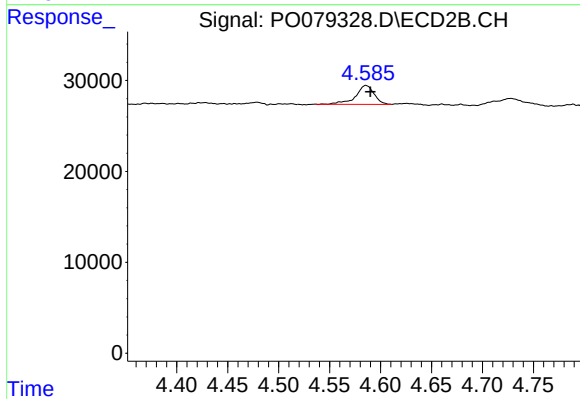

#9 AR-1221-2


R.T.: 4.586 min
Delta R.T.: -0.005 min
Response: 26373
Conc: 101.37 ng/ml

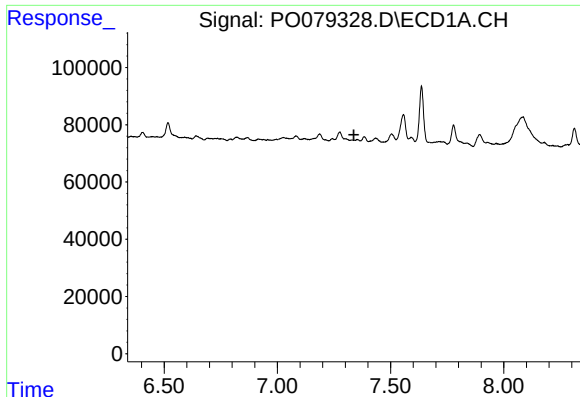

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

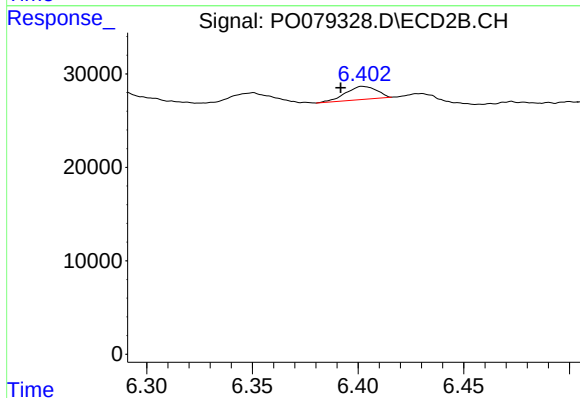


#20 AR-1242-5

R.T.: 6.402 min
Delta R.T.: 0.010 min
Response: 14241
Conc: 18.96 ng/ml

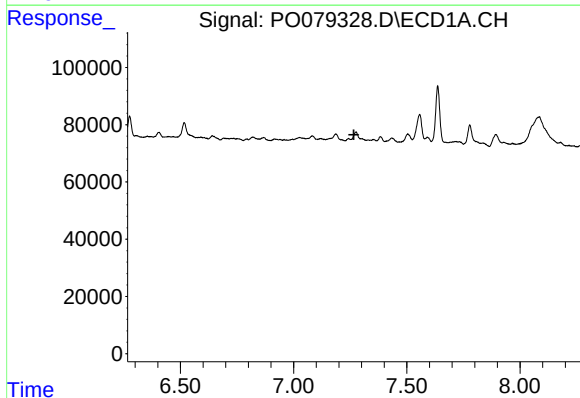


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.266 min
Response: 0
Conc: N.D.

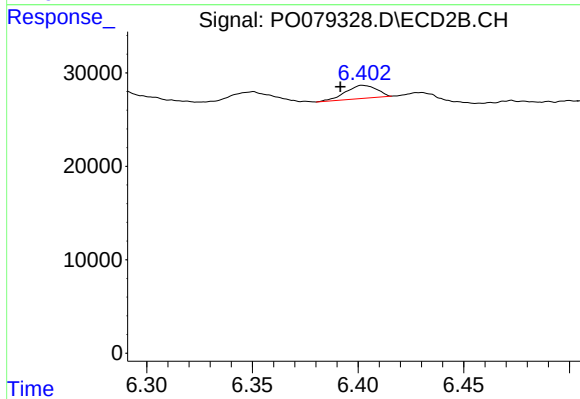

#26 AR-1254-1


R.T.: 6.402 min
Delta R.T.: 0.011 min
Response: 14241
Conc: 8.92 ng/ml

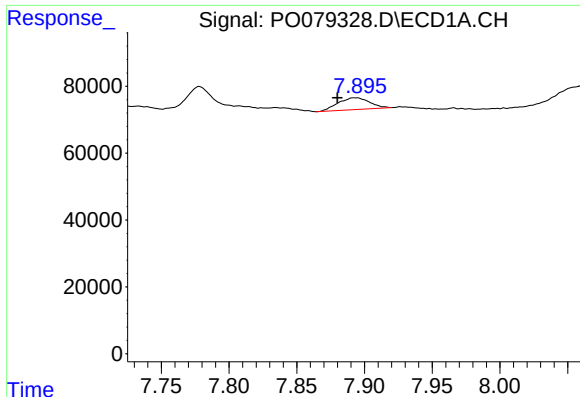

#28 AR-1254-3


R.T.: 7.893 min
Delta R.T.: 0.014 min
Response: 56929
Conc: 16.10 ng/ml

Instrument :
ECD_O
ClientSampleId :

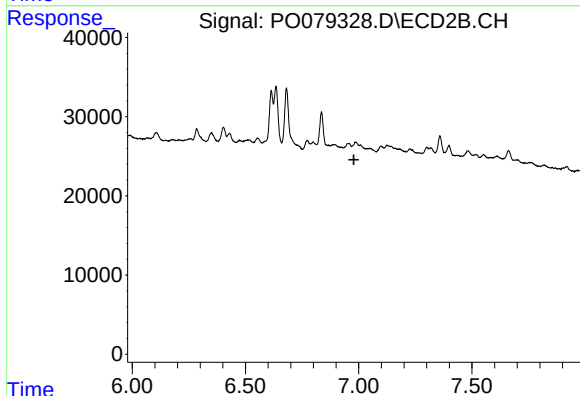


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.979 min
Response: 0
Conc: N.D.

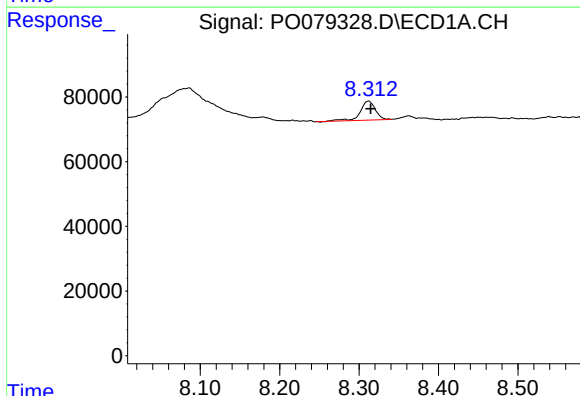


#32 AR-1260-2

R.T.: 8.312 min
Delta R.T.: -0.003 min
Response: 77142
Conc: 28.06 ng/ml

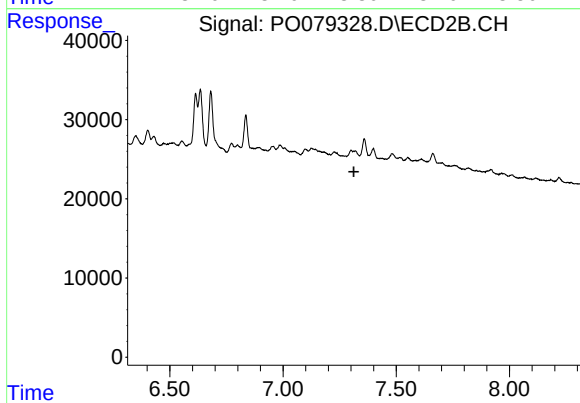

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.313 min
Response: 0
Conc: N.D.

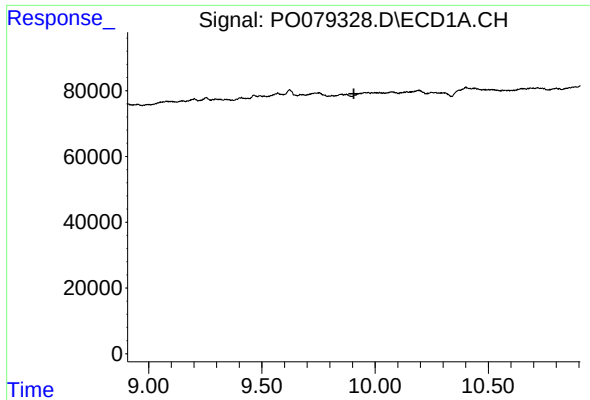

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.906 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

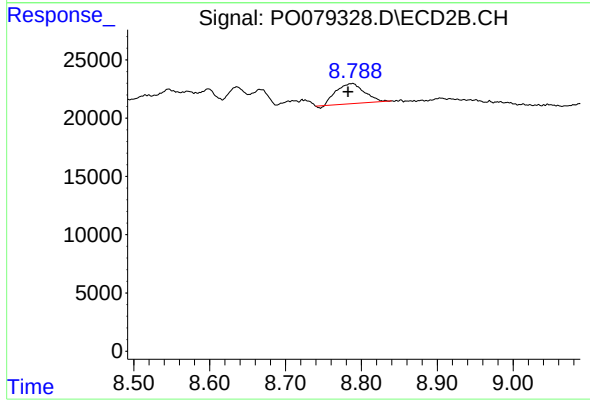

#43 AR-1268-3

R.T.: 8.789 min
Delta R.T.: 0.006 min
Response: 44754
Conc: 17.39 ng/ml