

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 22:16
Operator : DD\AJ
Sample : M2933-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:42:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.227	1478833	673226	25.378	22.885
2) SA Decachlor...	11.146	9.670	1088665	567812	25.778	21.706

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 22:16
Operator : DD\AJ
Sample : M2933-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:42:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

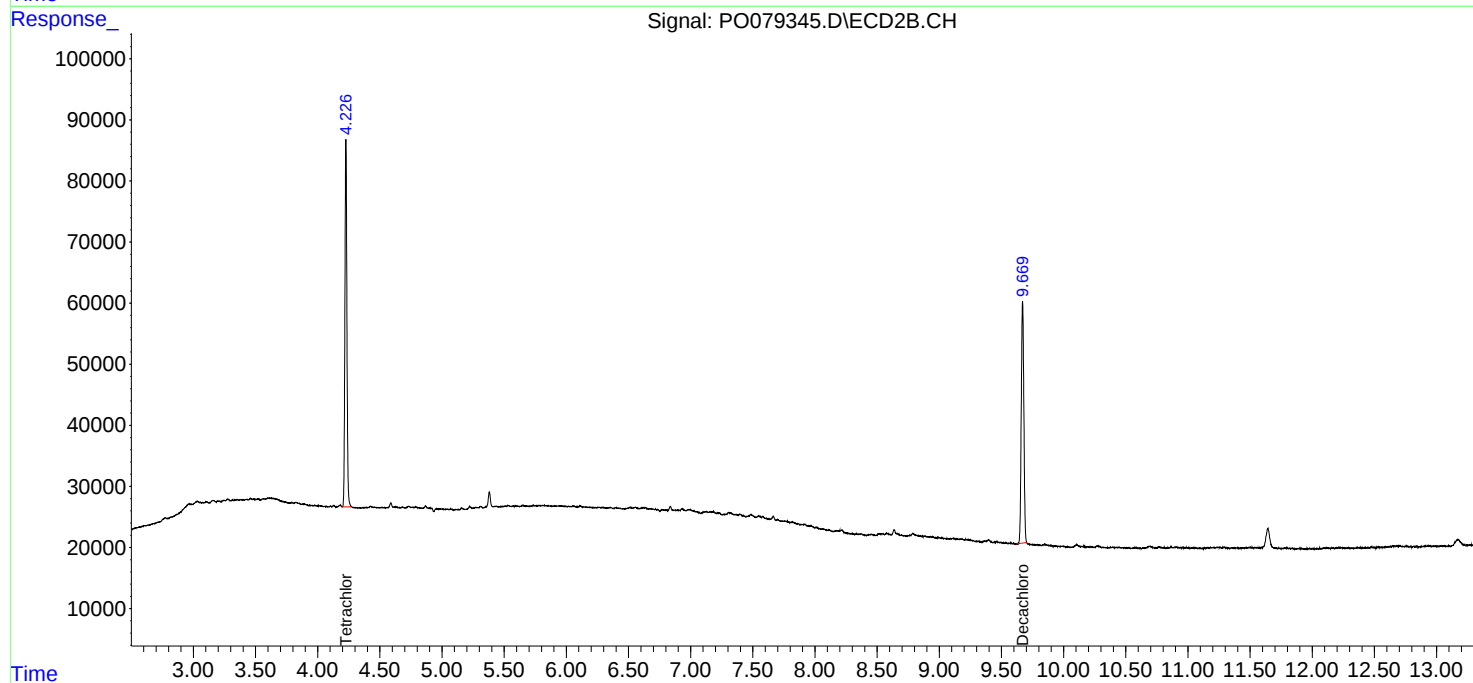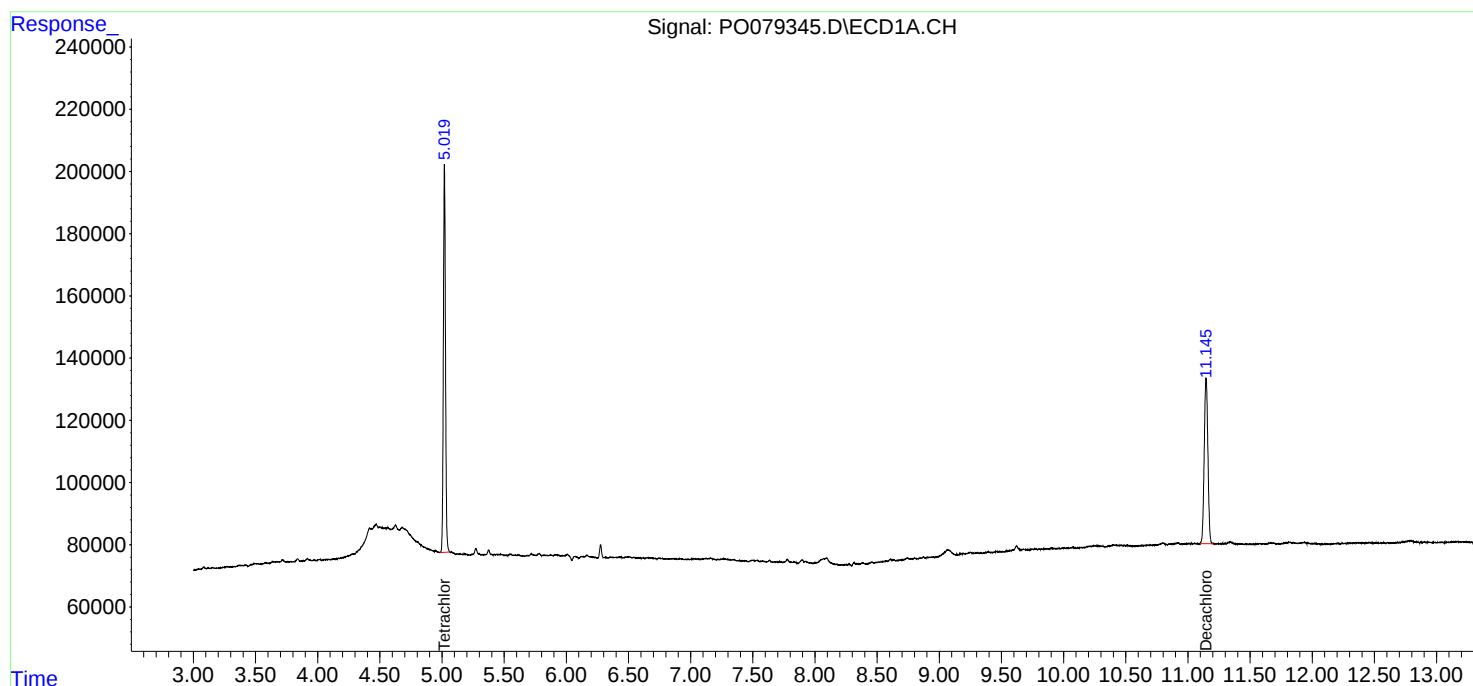


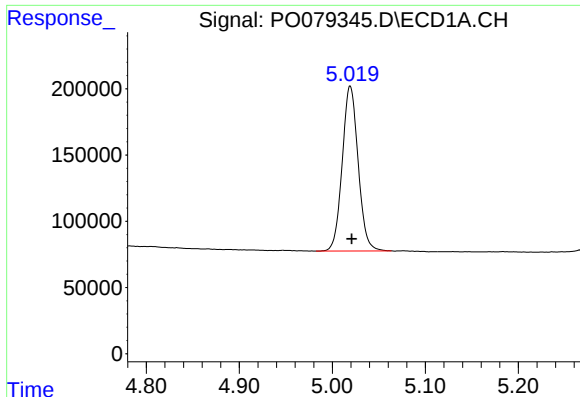

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 1478833
Conc: 25.38 ng/ml

Instrument :
ECD_O
ClientSampleId :

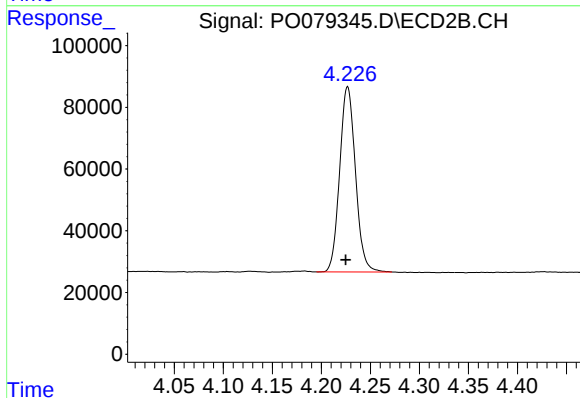


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: 0.002 min
Response: 673226
Conc: 22.88 ng/ml

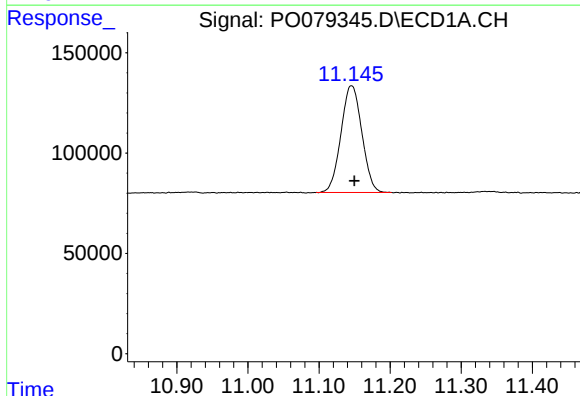

#2 Decachlorobiphenyl

R.T.: 11.146 min
Delta R.T.: -0.004 min
Response: 1088665
Conc: 25.78 ng/ml

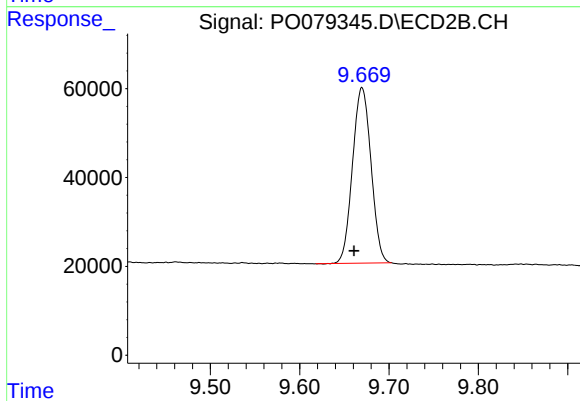

#2 Decachlorobiphenyl

R.T.: 9.670 min
Delta R.T.: 0.009 min
Response: 567812
Conc: 21.71 ng/ml