

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
 Data File : P0079356.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jul 2021 2:02
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 04:45:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 02 07:33:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.019	4.228	1302277	589078	22.348	20.025
2)	SA Decachlor...	11.147	9.672	1024952	529109	24.269	20.227

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079356.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jul 2021 2:02
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:45:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

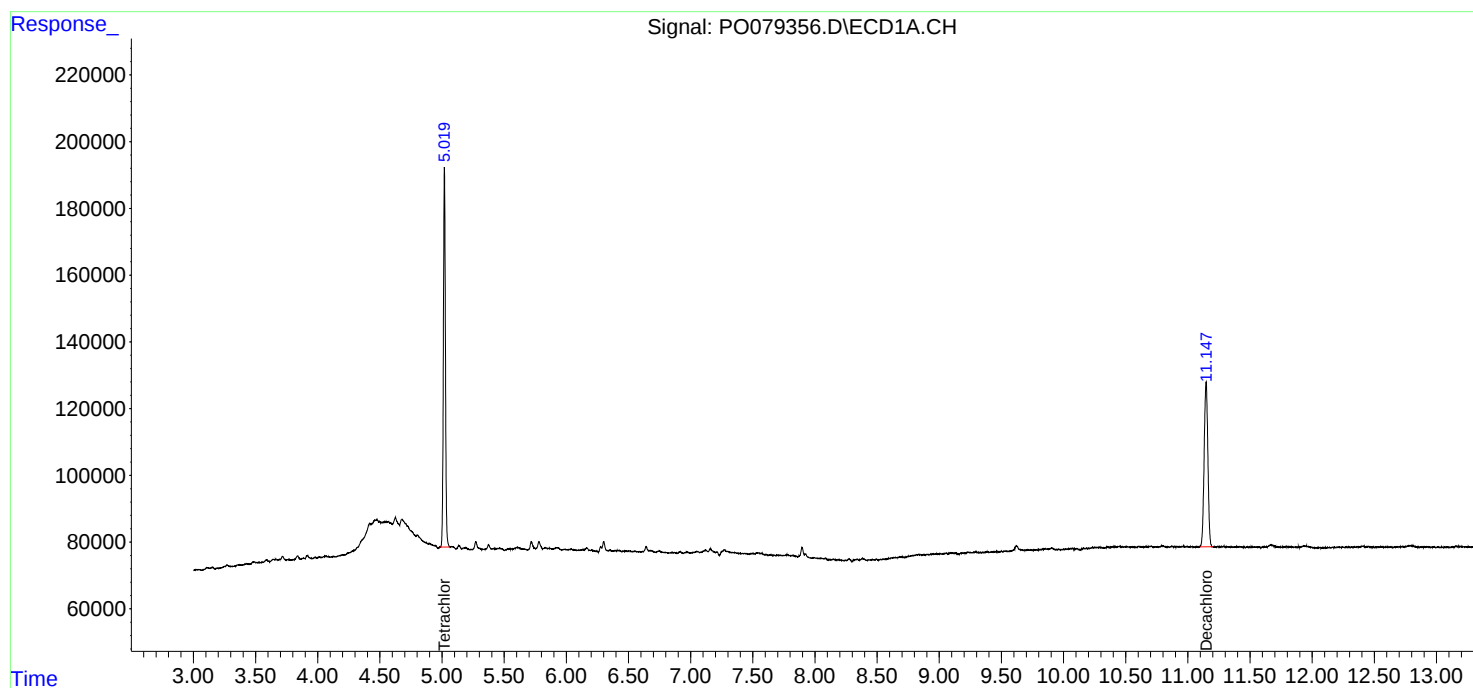


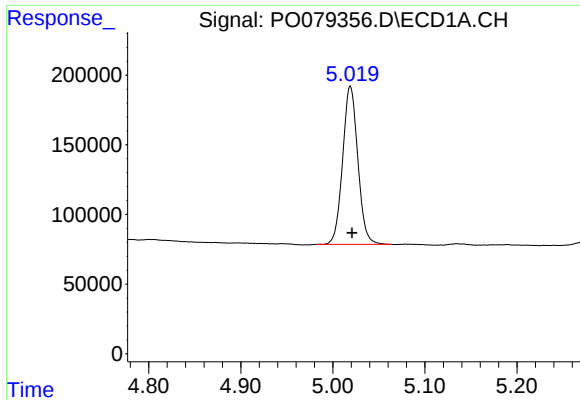

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 1302277
Conc: 22.35 ng/ml

Instrument :
ECD_O
ClientSampleId :

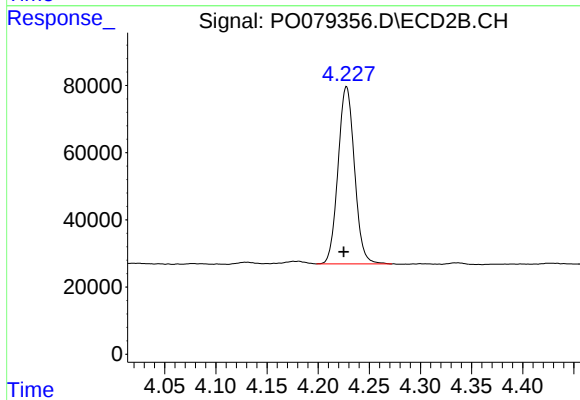


#1 Tetrachloro-m-xylene

R.T.: 4.228 min
Delta R.T.: 0.003 min
Response: 589078
Conc: 20.02 ng/ml

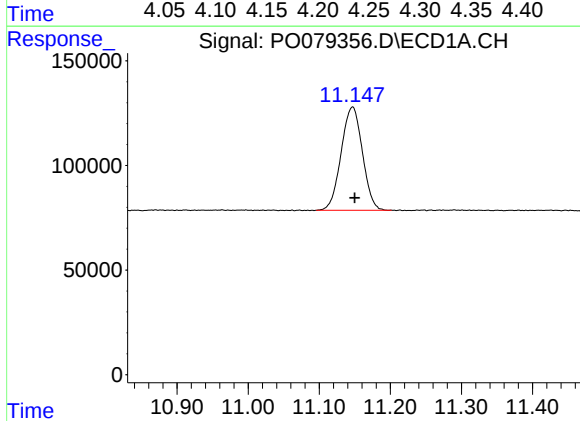

#2 Decachlorobiphenyl

R.T.: 11.147 min
Delta R.T.: -0.003 min
Response: 1024952
Conc: 24.27 ng/ml

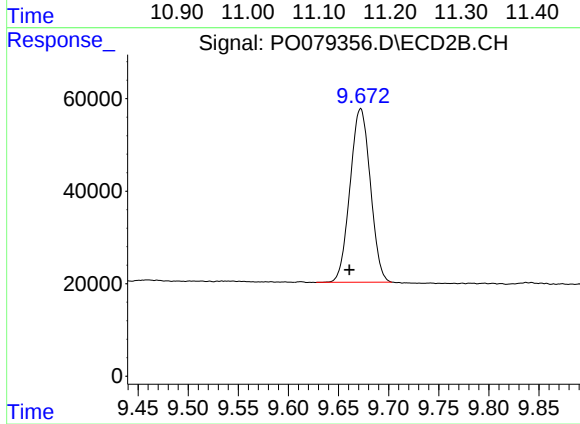

#2 Decachlorobiphenyl

R.T.: 9.672 min
Delta R.T.: 0.011 min
Response: 529109
Conc: 20.23 ng/ml