

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
 Data File : P0079358.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jul 2021 2:37
 Operator : DD\AJ
 Sample : M2937-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 04:45:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 02 07:33:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.020	4.229	1400021	666726	24.026	22.664
2) SA Decachlor...	11.146	9.672	1131044	568920	26.781	21.749
Target Compounds						
30) L6 AR-1254-5	8.606	0.000	80612	0	30.344	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079358.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jul 2021 2:37
Operator : DD\AJ
Sample : M2937-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:45:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

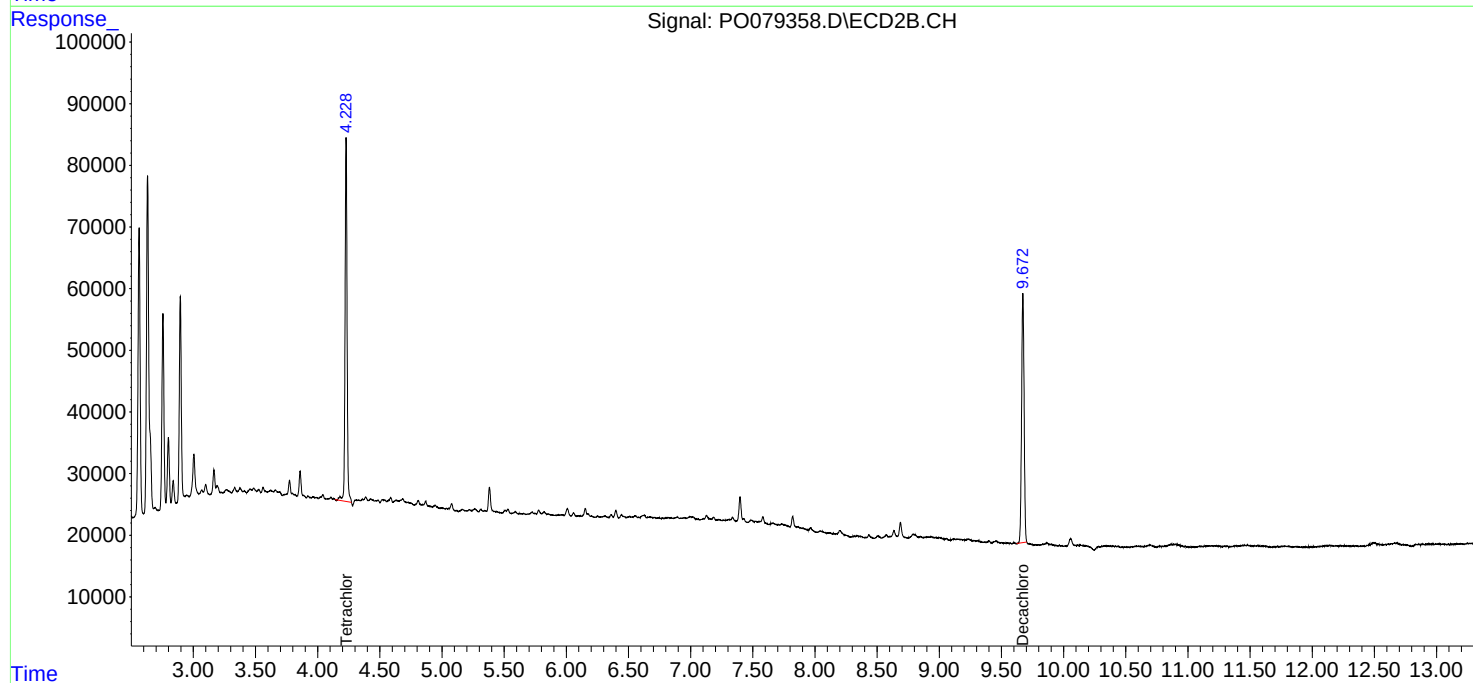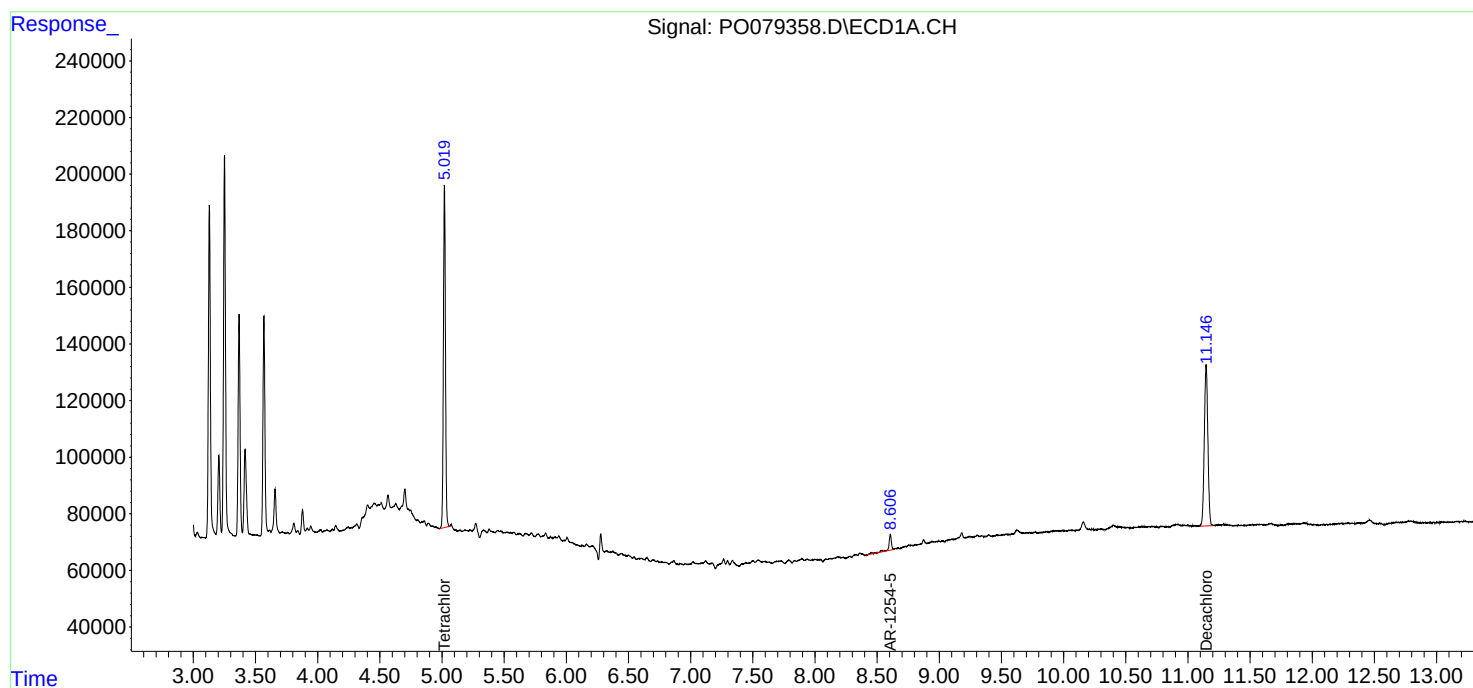


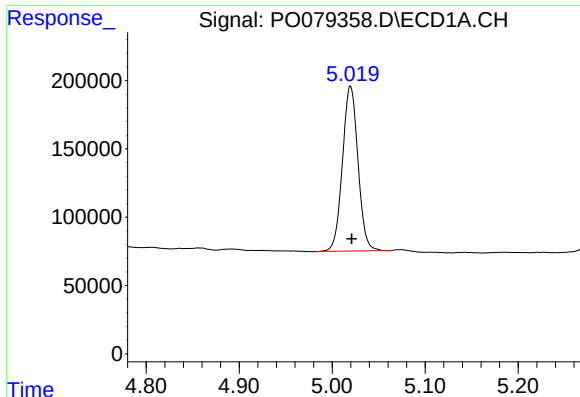

#1 Tetrachloro-m-xylene


R.T.: 5.020 min
Delta R.T.: -0.001 min
Response: 1400021
Conc: 24.03 ng/ml

Instrument :
ECD_O
ClientSampleId :

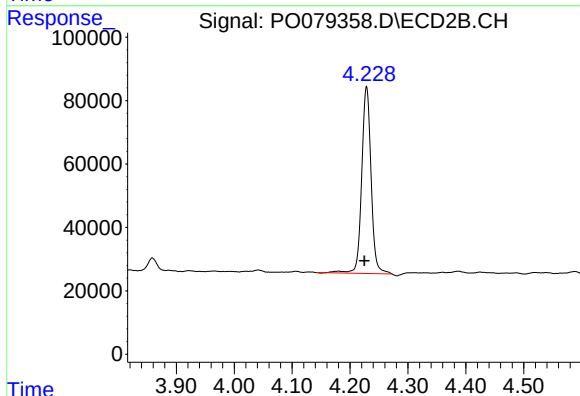


#1 Tetrachloro-m-xylene

R.T.: 4.229 min
Delta R.T.: 0.004 min
Response: 666726
Conc: 22.66 ng/ml

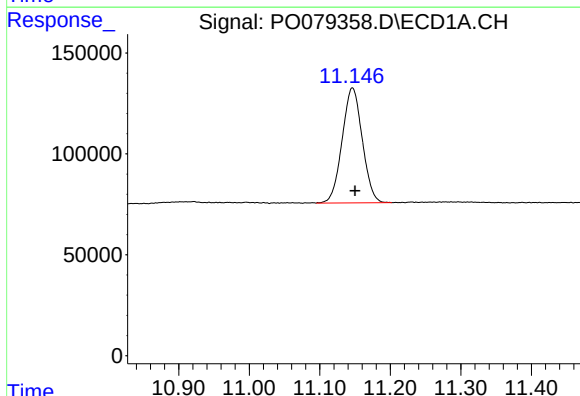


#2 Decachlorobiphenyl

R.T.: 11.146 min
Delta R.T.: -0.004 min
Response: 1131044
Conc: 26.78 ng/ml

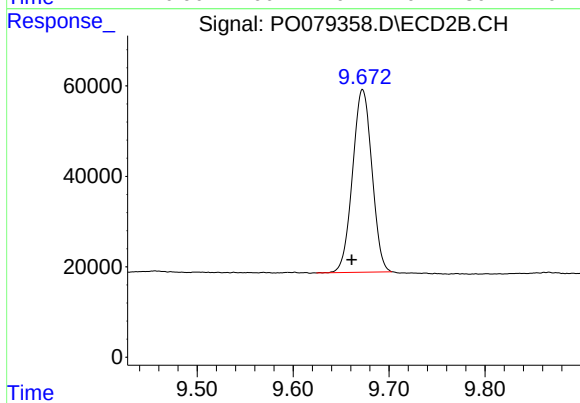

#2 Decachlorobiphenyl


R.T.: 9.672 min
Delta R.T.: 0.011 min
Response: 568920
Conc: 21.75 ng/ml

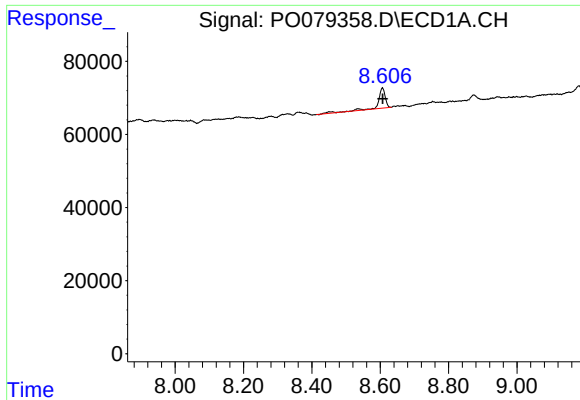

#30 AR-1254-5

R.T.: 8.606 min
Delta R.T.: -0.001 min
Response: 80612
Conc: 30.34 ng/ml

Instrument :
ECD_O
ClientSampleId :

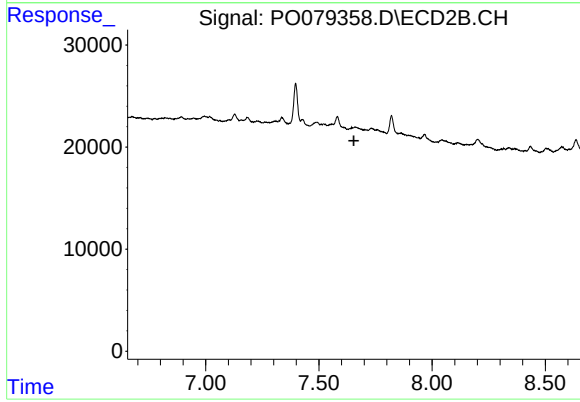

#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.654 min
Response: 0
Conc: N.D.