

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
 Data File : P0079317.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2021 13:15
 Operator : DD\AJ
 Sample : M2851-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-08

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 02:26:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 02 07:33:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.020	4.225	1408158	639557	24.165	21.740
2) SA Decachlor...	11.147	9.666	1031139	528358	24.415	20.198

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079317.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 13:15
Operator : DD\AJ
Sample : M2851-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 02:26:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

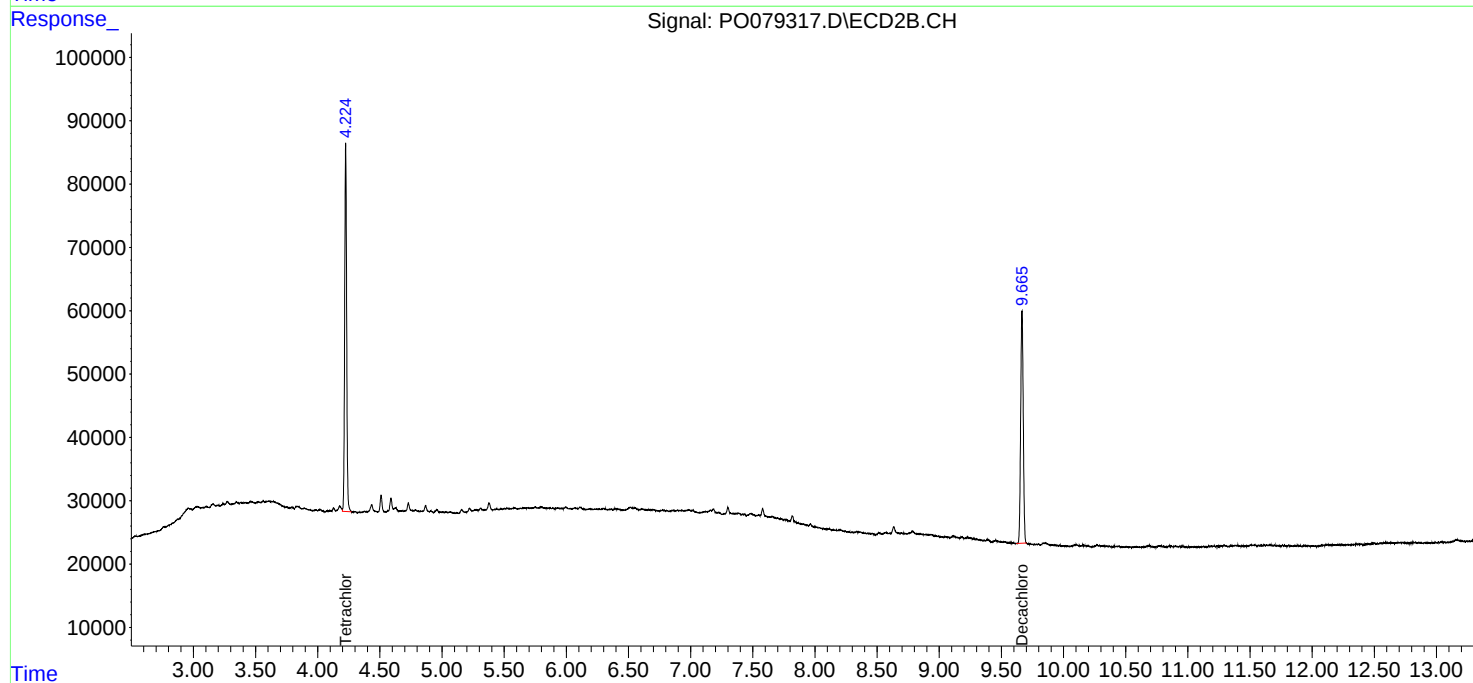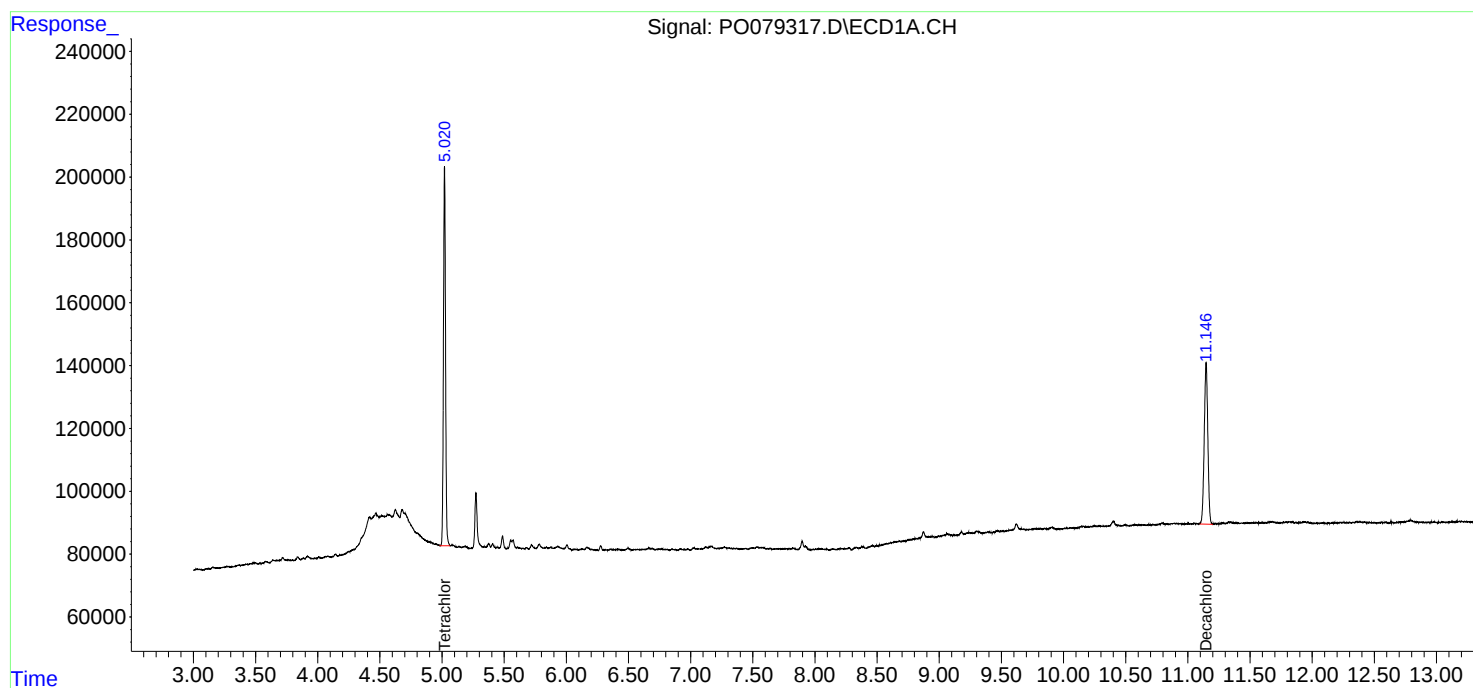


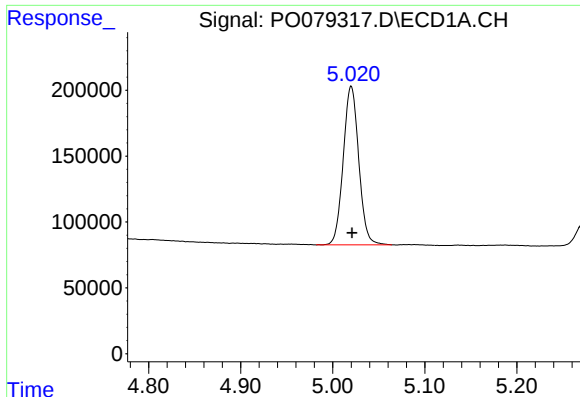

#1 Tetrachloro-m-xylene


R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 1408158
Conc: 24.17 ng/ml

Instrument :
ECD_O
ClientSampleId :
BACKFILL-ASHCROFT-REAR-08

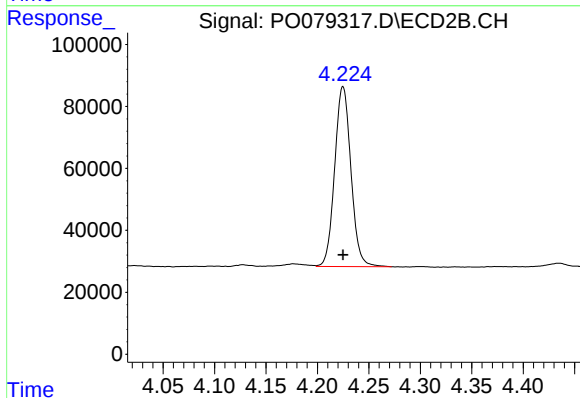


#1 Tetrachloro-m-xylene

R.T.: 4.225 min
Delta R.T.: 0.000 min
Response: 639557
Conc: 21.74 ng/ml

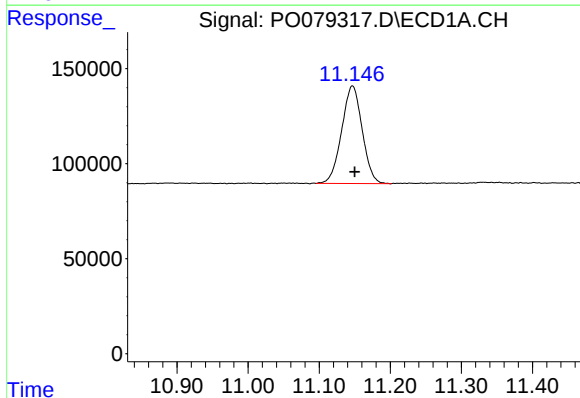

#2 Decachlorobiphenyl

R.T.: 11.147 min
Delta R.T.: -0.003 min
Response: 1031139
Conc: 24.42 ng/ml

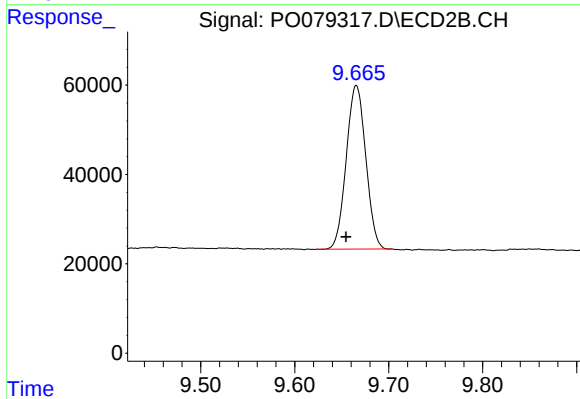

#2 Decachlorobiphenyl

R.T.: 9.666 min
Delta R.T.: 0.011 min
Response: 528358
Conc: 20.20 ng/ml