

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079341.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 21:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:42:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.227	1246247	577336	21.387	19.625
2) SA Decachlor...	11.147	9.671	949215	496171	22.476	18.968

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079341.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 21:07
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:42:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

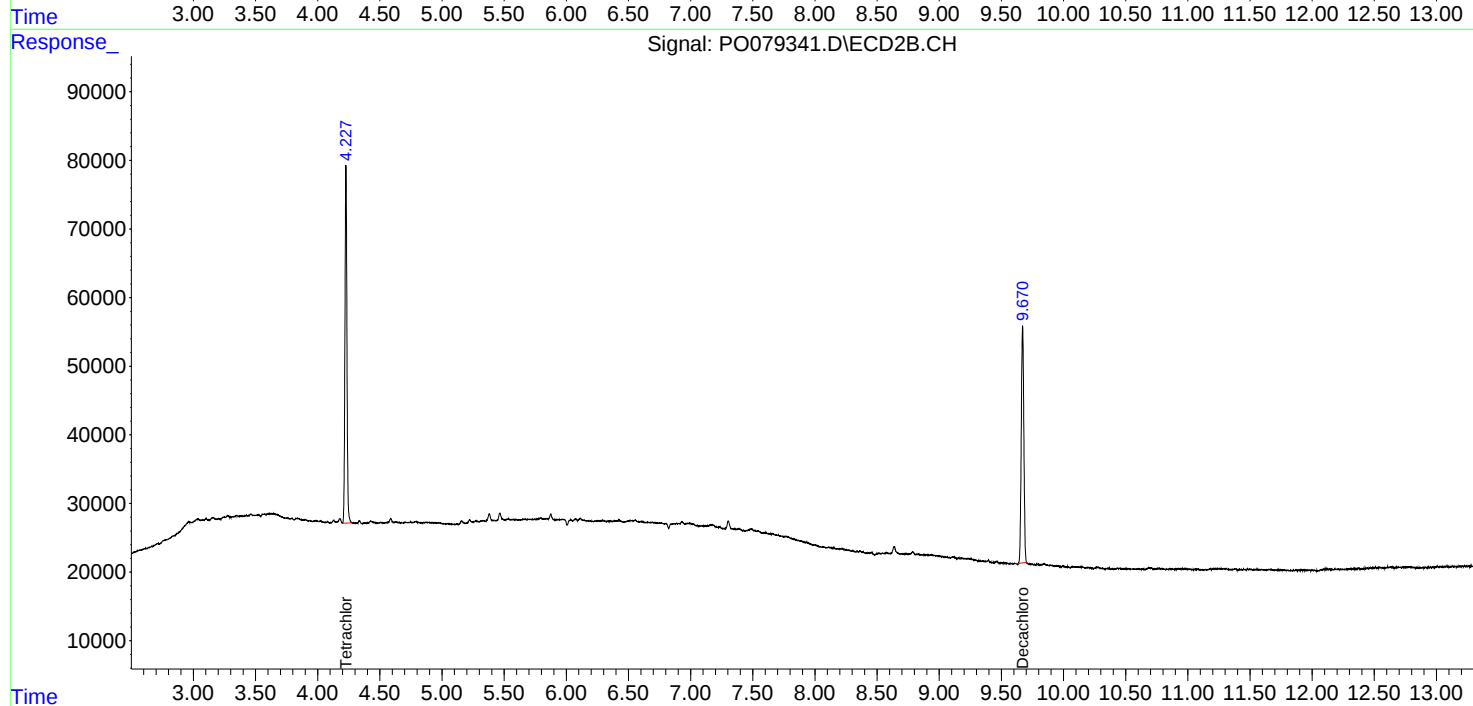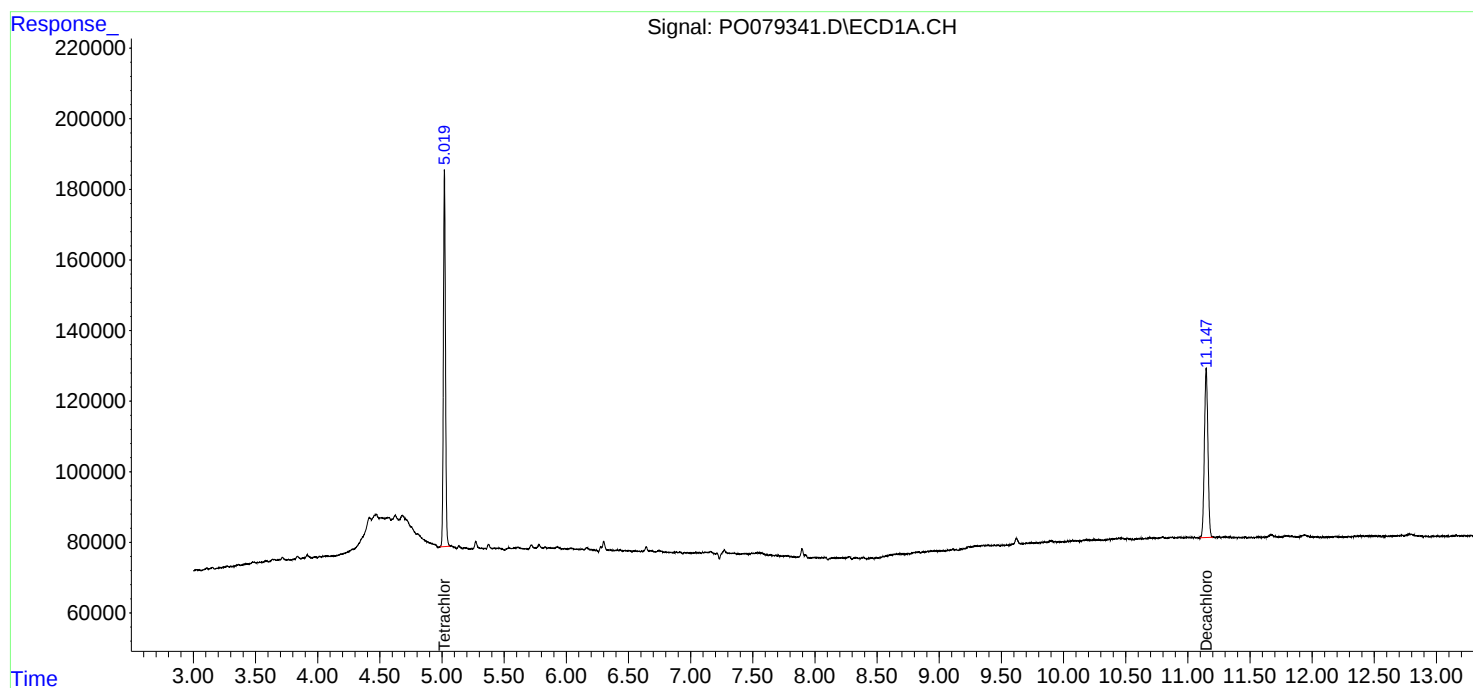


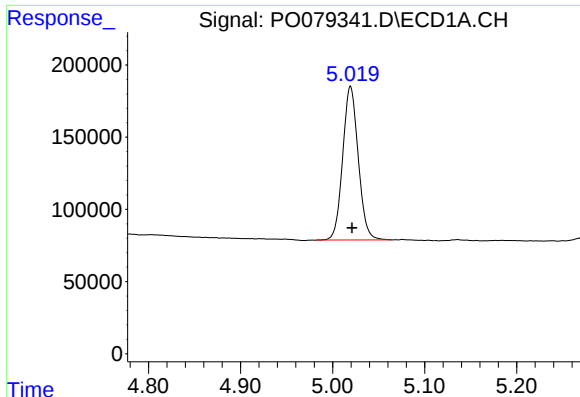

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.002 min
Response: 1246247
Conc: 21.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

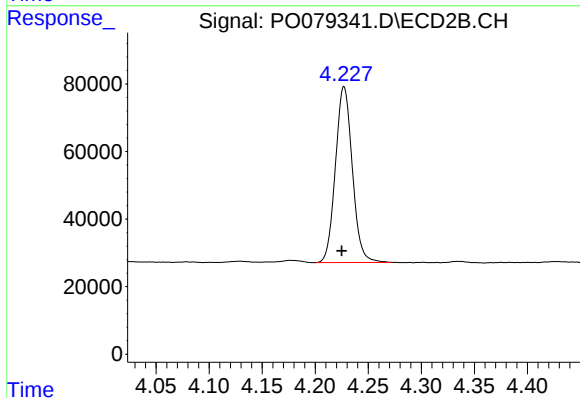


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: 0.002 min
Response: 577336
Conc: 19.63 ng/ml

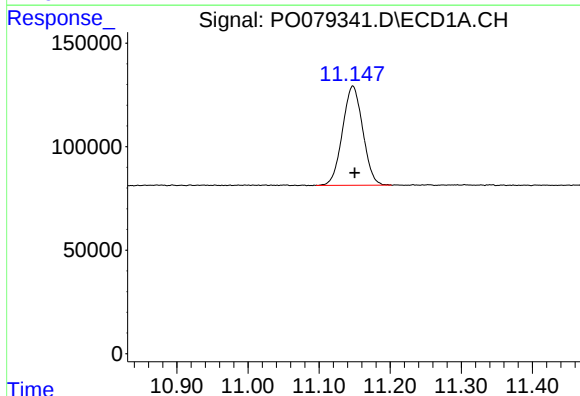

#2 Decachlorobiphenyl

R.T.: 11.147 min
Delta R.T.: -0.003 min
Response: 949215
Conc: 22.48 ng/ml

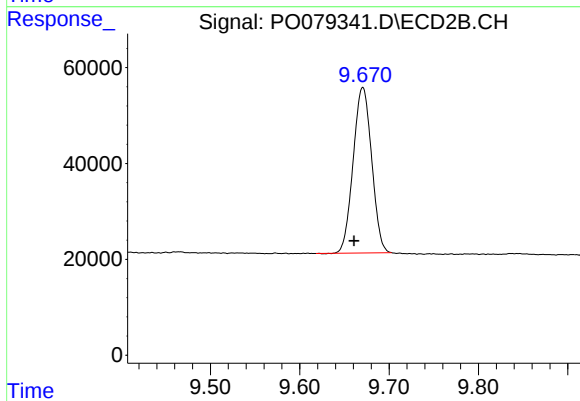

#2 Decachlorobiphenyl

R.T.: 9.671 min
Delta R.T.: 0.010 min
Response: 496171
Conc: 18.97 ng/ml