

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
 Data File : P0079348.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Jul 2021 23:09
 Operator : DD\AJ
 Sample : M2927-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1132

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 04:43:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Jul 02 07:33:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.020	4.227	1419904	663453	24.367	22.553
2) SA Decachlor...	11.146	9.672	1069761	535331	25.330	20.465

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070621\
Data File : P0079348.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Jul 2021 23:09
Operator : DD\AJ
Sample : M2927-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AUD-1132

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 04:43:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Jul 02 07:33:59 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

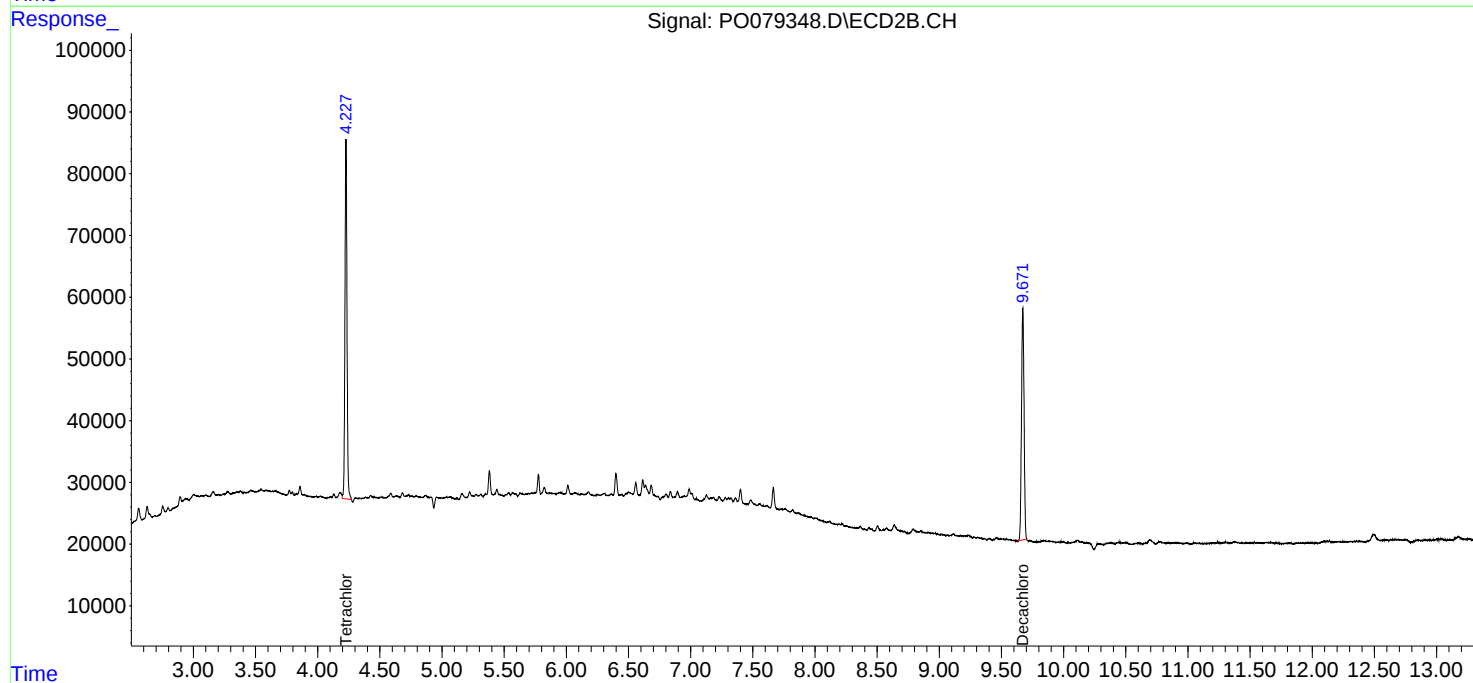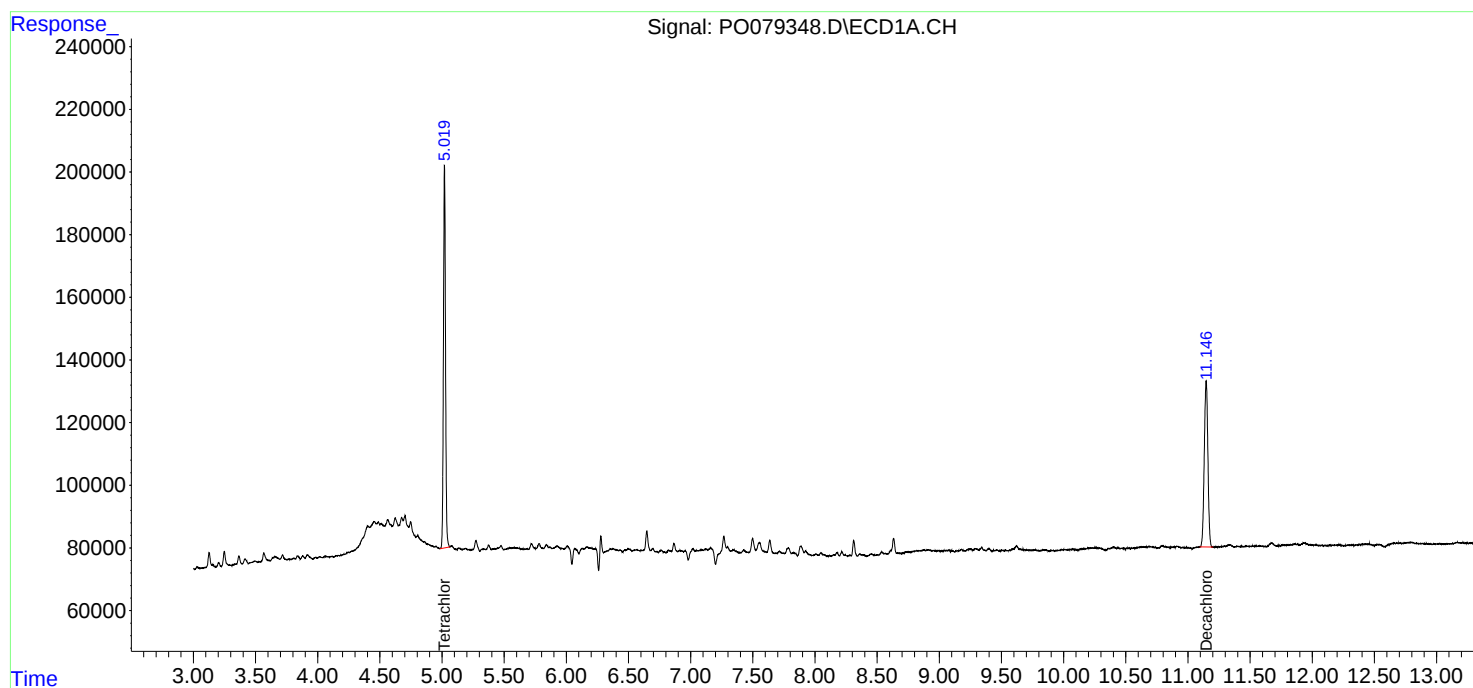


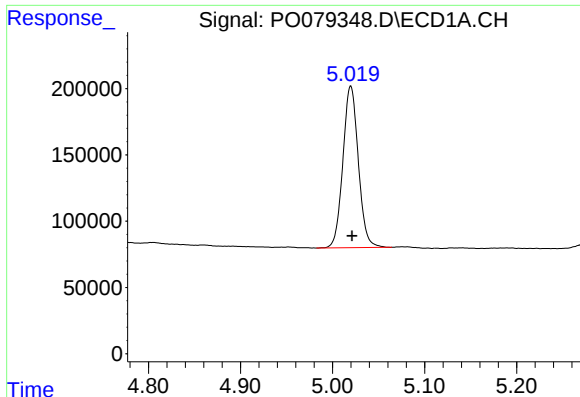

#1 Tetrachloro-m-xylene


R.T.: 5.020 min
Delta R.T.: -0.001 min
Response: 1419904
Conc: 24.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1132

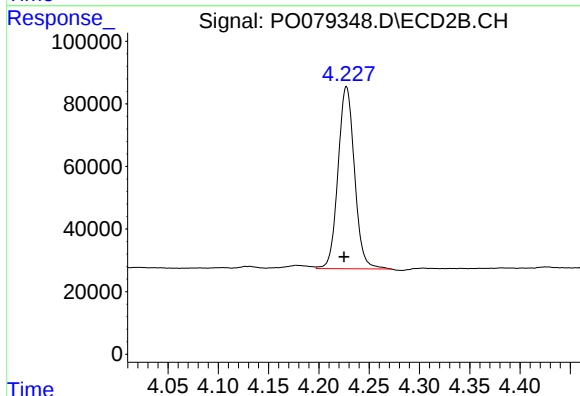


#1 Tetrachloro-m-xylene

R.T.: 4.227 min
Delta R.T.: 0.002 min
Response: 663453
Conc: 22.55 ng/ml

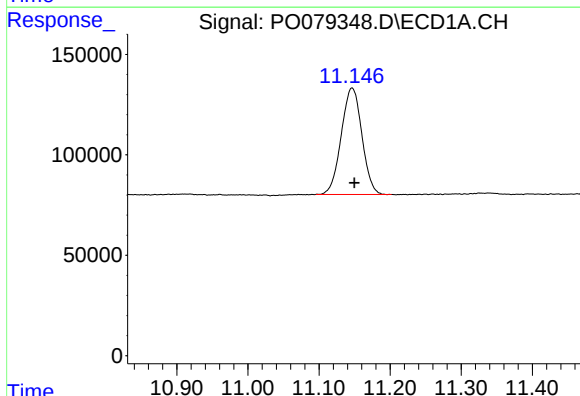

#2 Decachlorobiphenyl

R.T.: 11.146 min
Delta R.T.: -0.004 min
Response: 1069761
Conc: 25.33 ng/ml

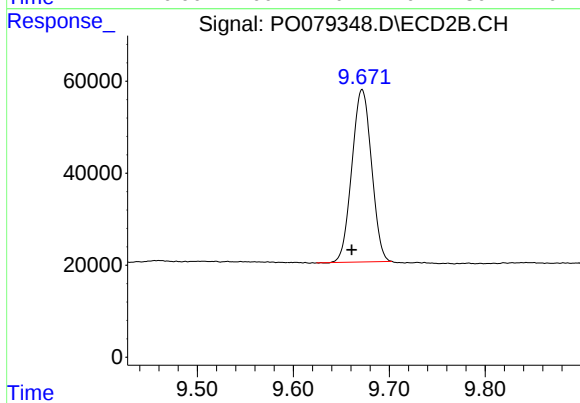

#2 Decachlorobiphenyl

R.T.: 9.672 min
Delta R.T.: 0.011 min
Response: 535331
Conc: 20.46 ng/ml