

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070720\
 Data File : P0069422.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jul 2020 10:46
 Operator : DD\AJ
 Sample : L3175-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PRESS-SAMPLE

Manual Integrations
 APPROVED

Ankita
 7/8/2020 10:19:15 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:42:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.402	3.569	927689	1150844	31.359	29.900m
2) SA Decachlor...	10.073	8.787	986789	2747830	20.776m	50.478m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070720\
Data File : P0069422.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jul 2020 10:46
Operator : DD\AJ
Sample : L3175-01
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PRESS-SAMPLE


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:15 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:42:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

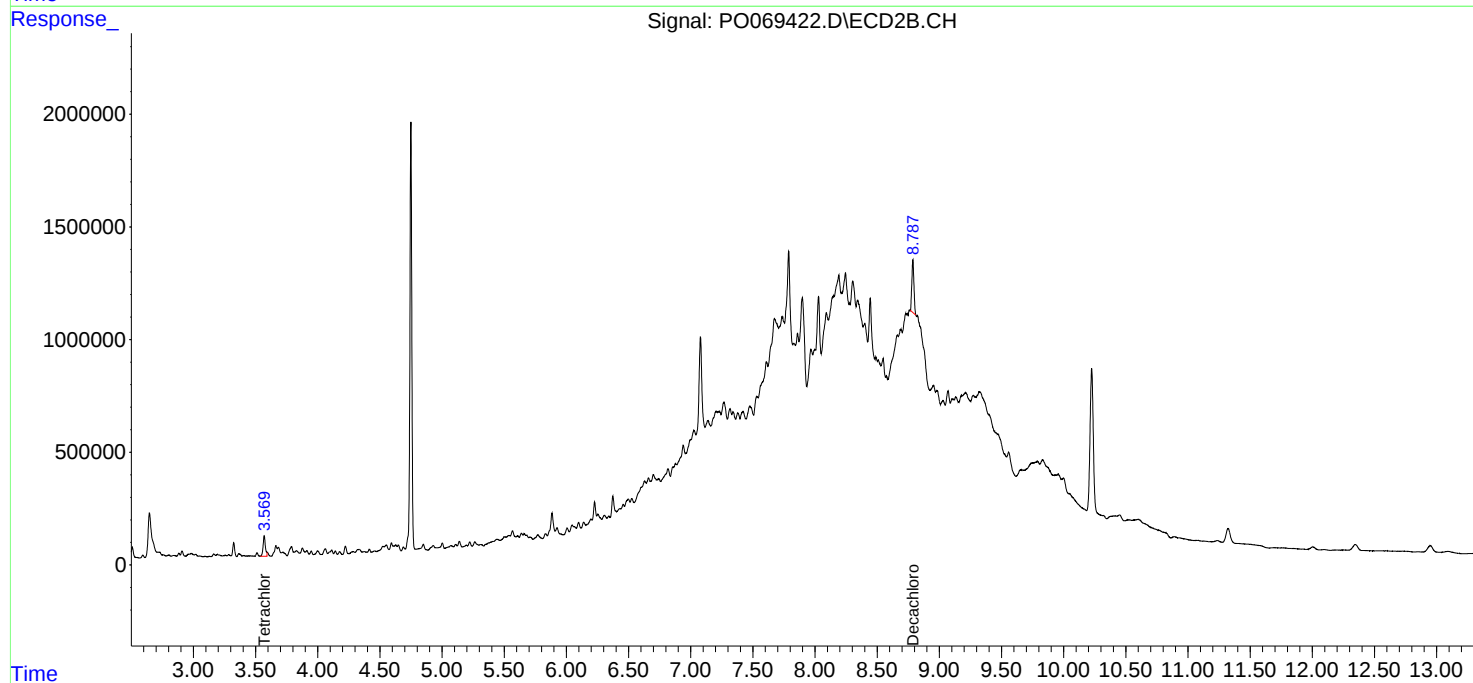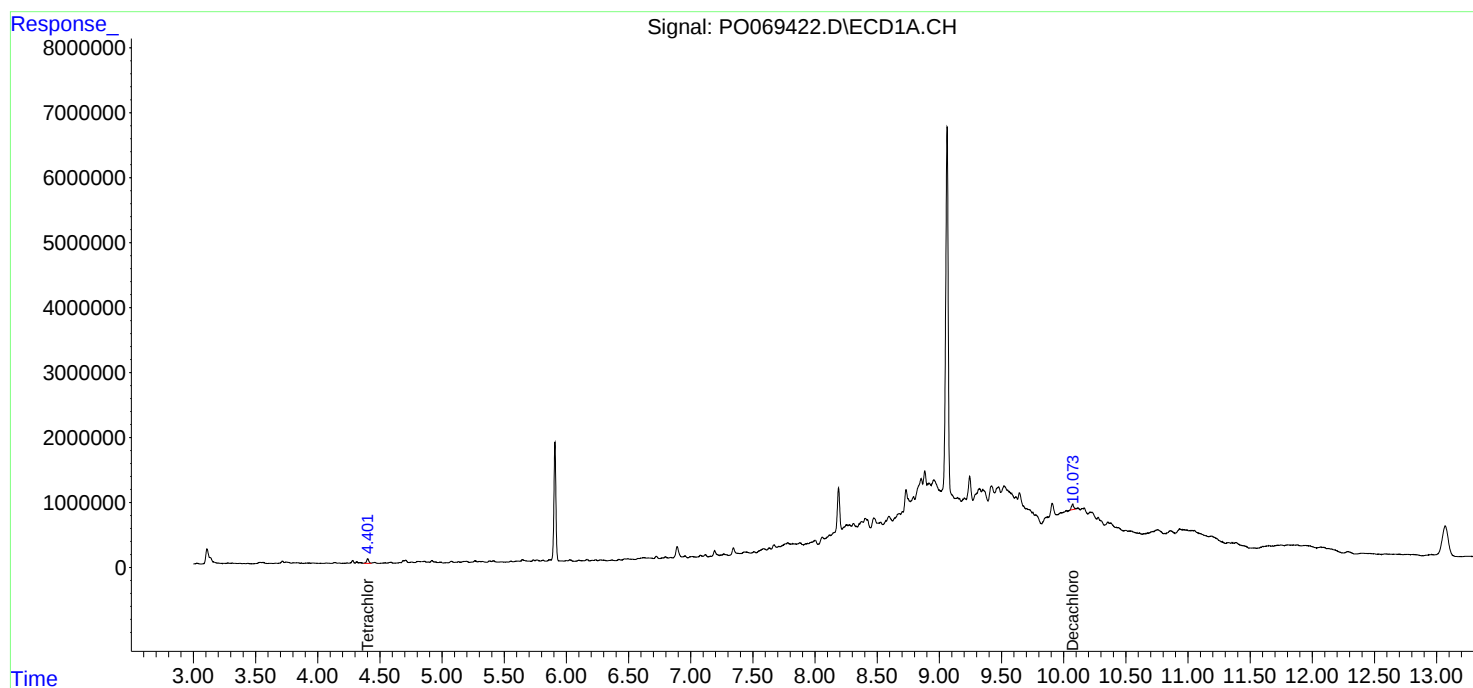

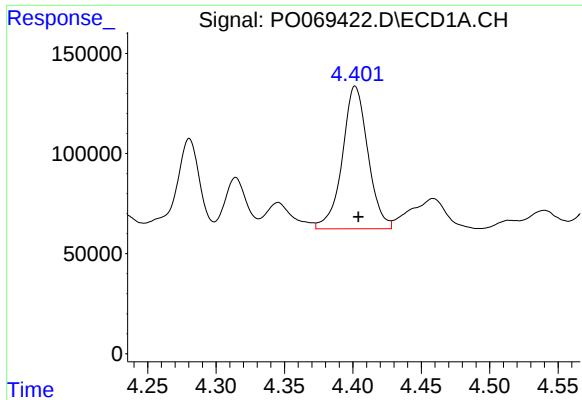


#1 Tetrachloro-m-xylene

R.T.: 4.402 min
Delta R.T.: -0.002 min
Response: 927689
Conc: 31.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
PRESS-SAMPLE


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:15 AM

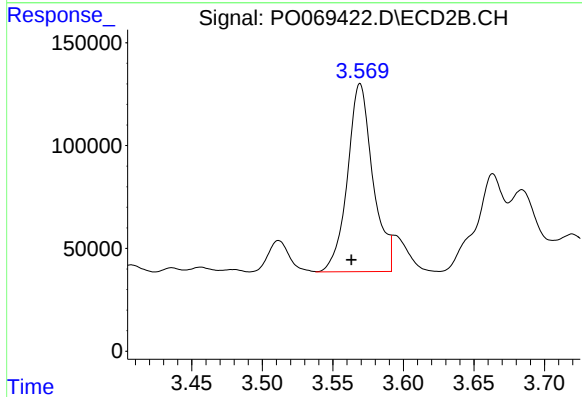


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.006 min
Response: 1150844
Conc: 29.90 ng/ml m

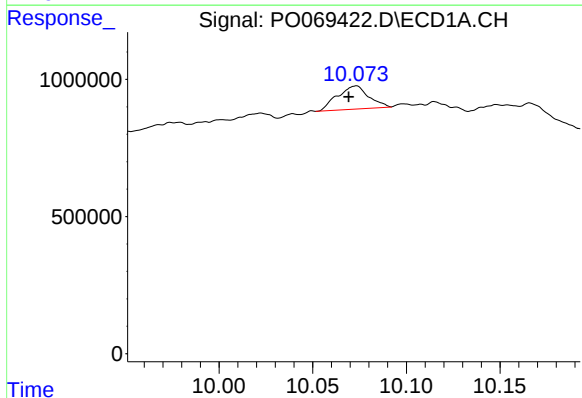

#2 Decachlorobiphenyl

R.T.: 10.073 min
Delta R.T.: 0.004 min
Response: 986789
Conc: 20.78 ng/ml m

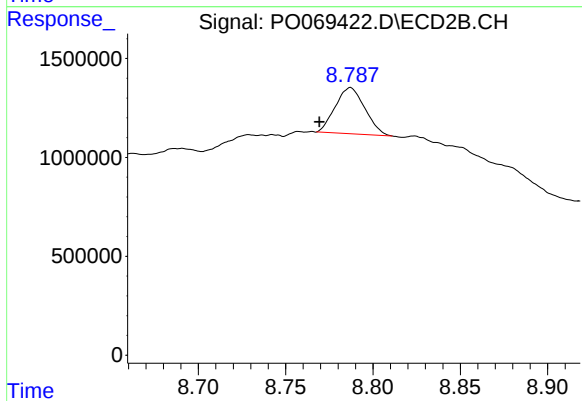

#2 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: 0.017 min
Response: 2747830
Conc: 50.48 ng/ml m