

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070720\
 Data File : P0069423.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jul 2020 11:03
 Operator : DD\AJ
 Sample : L3220-01 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-062220-SR-01

Manual Integrations
 APPROVED

Ankita
 7/8/2020 10:19:17 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 05:04:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.395	3.564	246745	170339	8.341	4.426 #
2)	SA Decachlor...	10.055	8.775	223388	201589	4.703m	3.703m
Target Compounds							
26)	L6 AR-1254-1	6.600	5.655	105229	186472	71.646	79.423
27)	L6 AR-1254-2	6.829	5.815	182946	103759	76.127	48.807 #
28)	L6 AR-1254-3	7.205	6.227	104120	109048	40.406	31.995
29)	L6 AR-1254-4	7.501	6.467	45794	53572	21.415	23.603m
30)	L6 AR-1254-5	7.918	6.891	253454	86911	121.180m	27.289m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070720\
Data File : PO069423.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jul 2020 11:03
Operator : DD\AJ
Sample : L3220-01 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-01


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:17 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 05:04:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

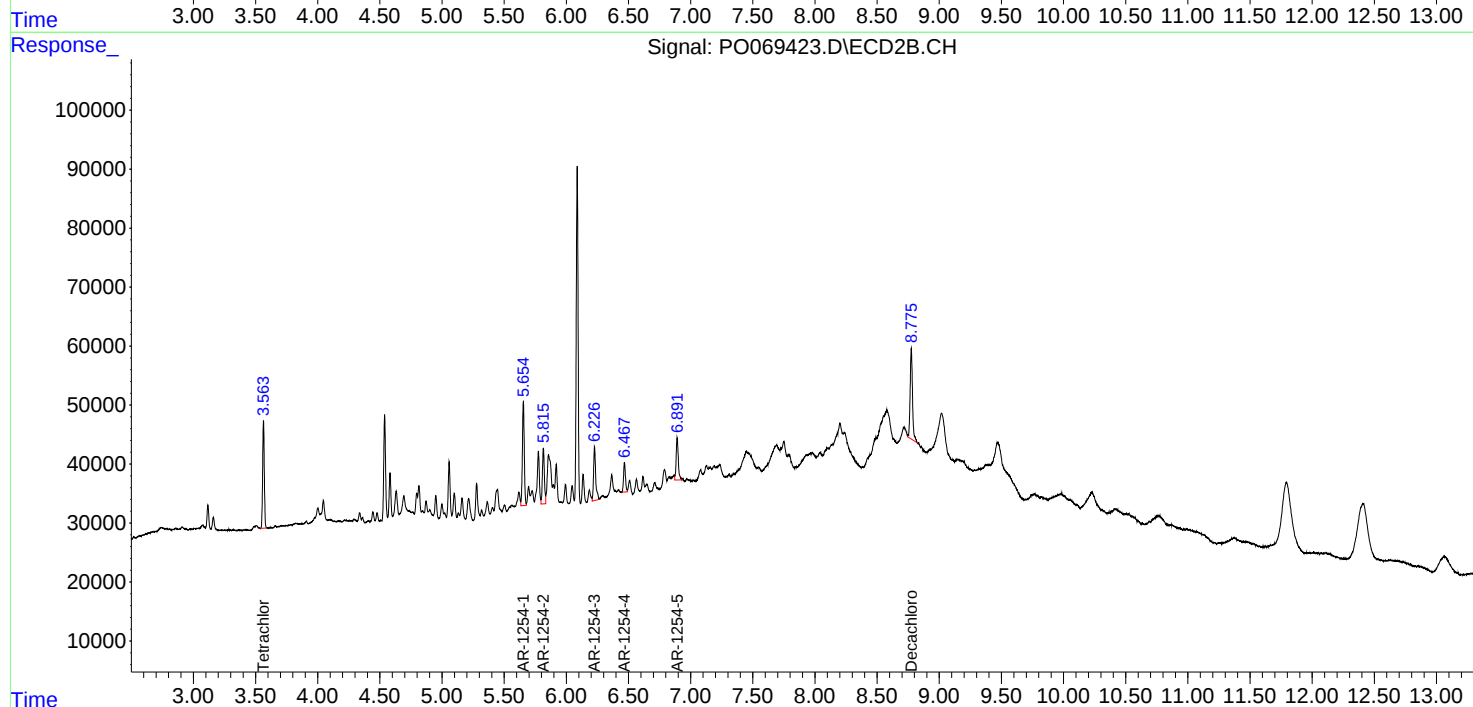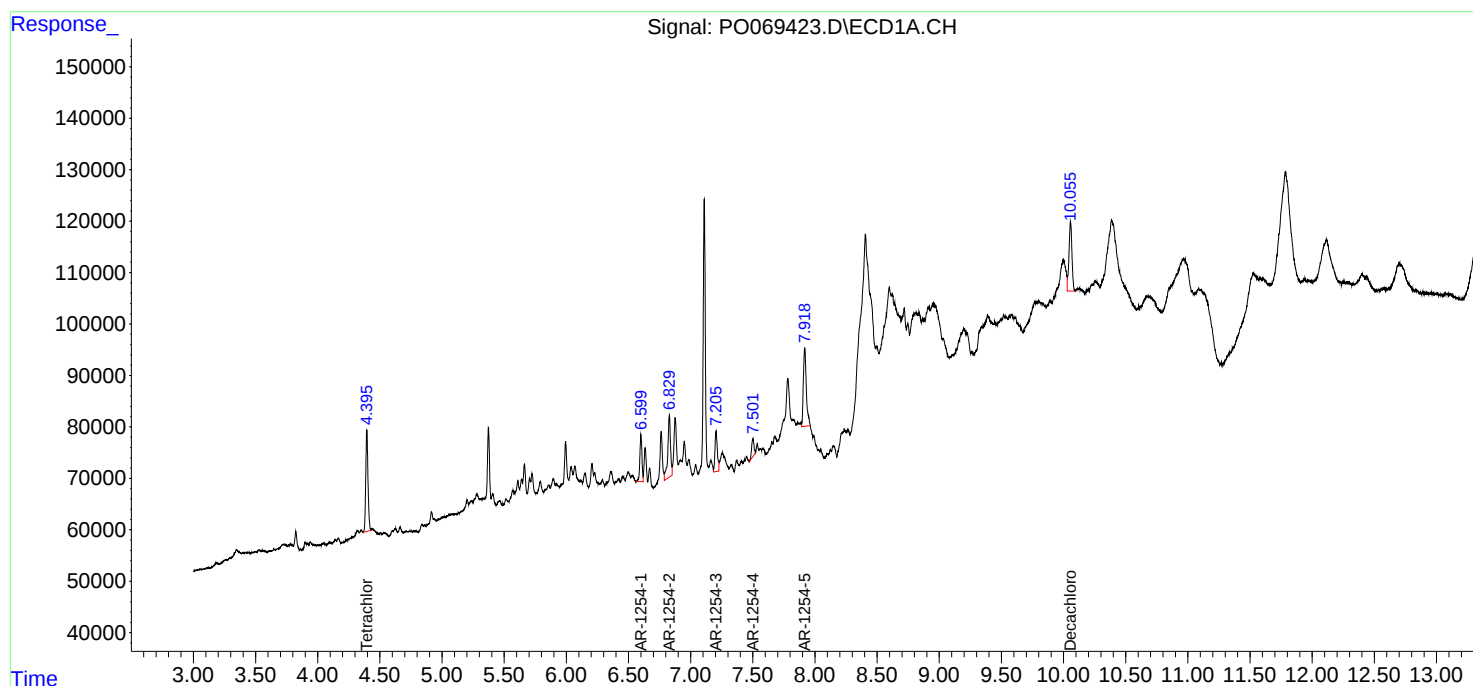

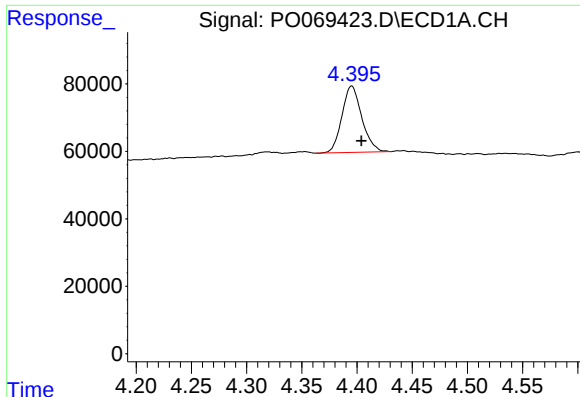


#1 Tetrachloro-m-xylene

R.T.: 4.395 min
Delta R.T.: -0.009 min
Response: 246745
Conc: 8.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-01


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:17 AM

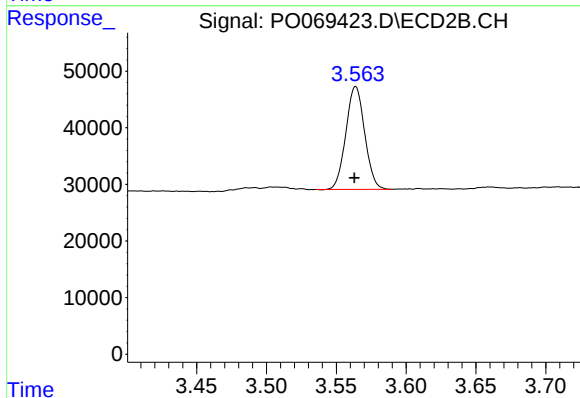


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.000 min
Response: 170339
Conc: 4.43 ng/ml

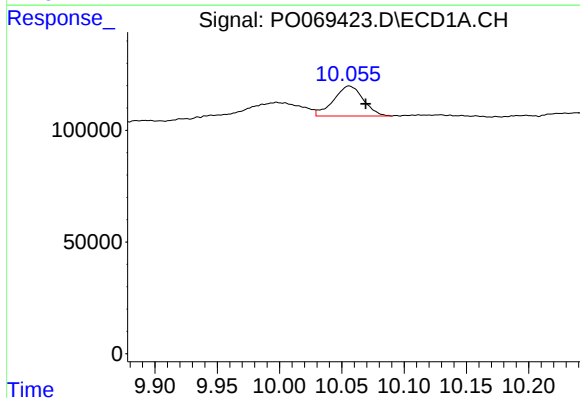


#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: -0.014 min
Response: 223388
Conc: 4.70 ng/ml m

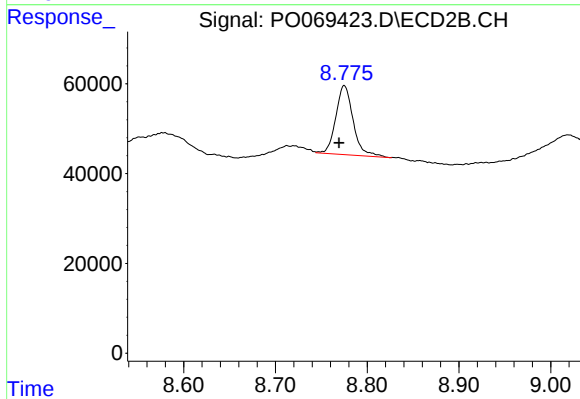

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: 0.005 min
Response: 201589
Conc: 3.70 ng/ml m

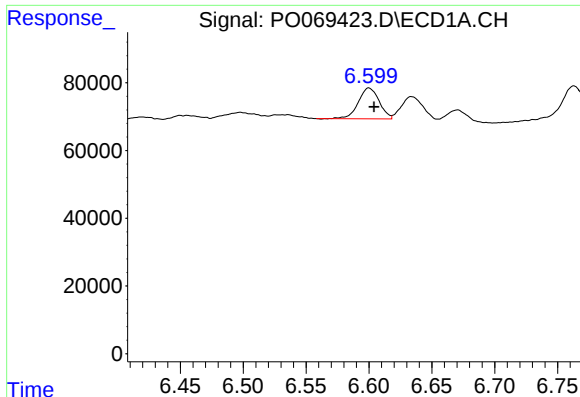


#26 AR-1254-1

R.T.: 6.600 min
Delta R.T.: -0.004 min
Response: 105229
Conc: 71.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-01


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:17 AM

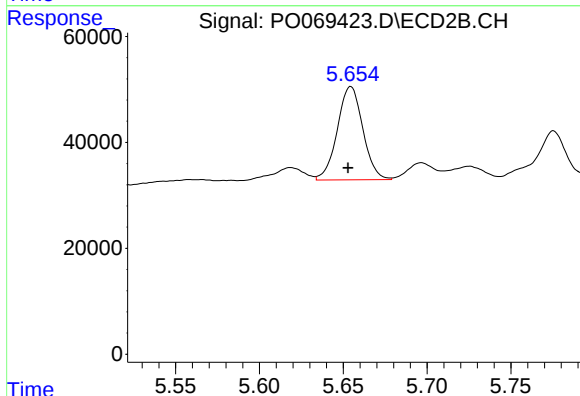


#26 AR-1254-1

R.T.: 5.655 min
Delta R.T.: 0.002 min
Response: 186472
Conc: 79.42 ng/ml

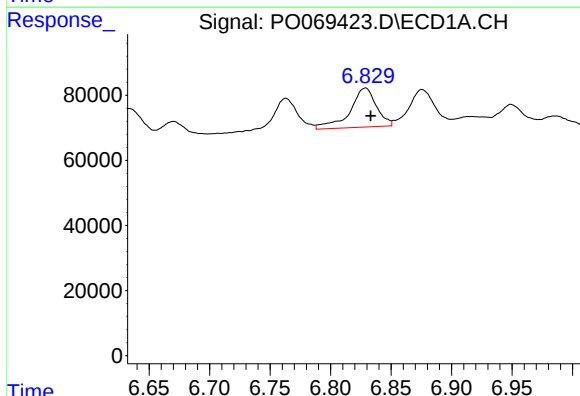


#27 AR-1254-2

R.T.: 6.829 min
Delta R.T.: -0.004 min
Response: 182946
Conc: 76.13 ng/ml

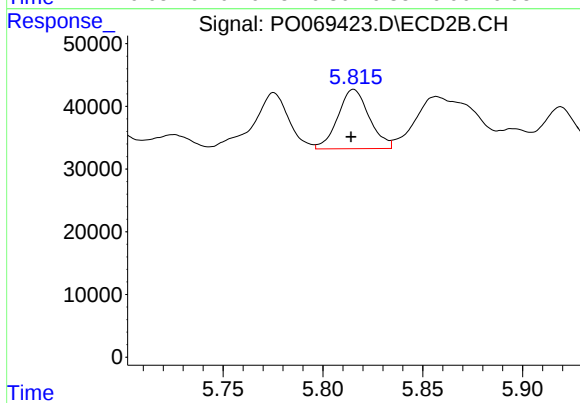

#27 AR-1254-2

R.T.: 5.815 min
Delta R.T.: 0.001 min
Response: 103759
Conc: 48.81 ng/ml

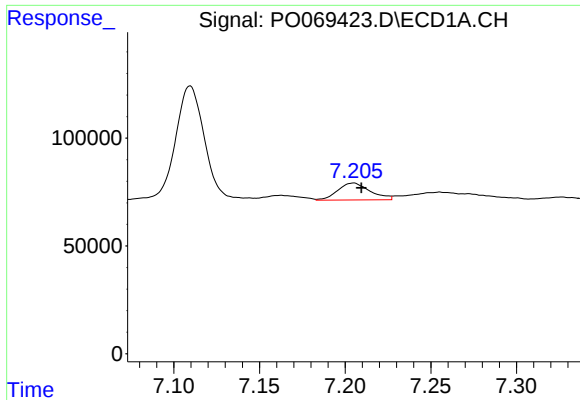


#28 AR-1254-3

R.T.: 7.205 min
Delta R.T.: -0.005 min
Response: 104120
Conc: 40.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-01


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:17 AM

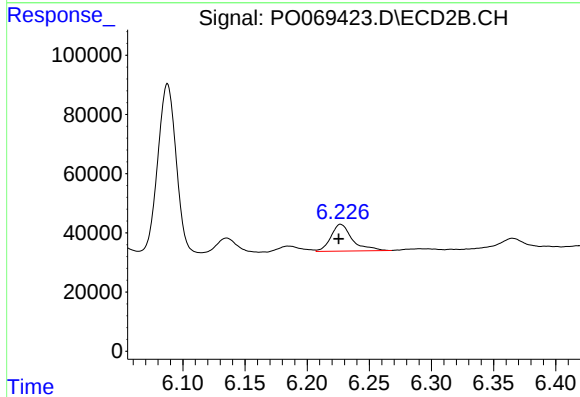


#28 AR-1254-3

R.T.: 6.227 min
Delta R.T.: 0.002 min
Response: 109048
Conc: 32.00 ng/ml

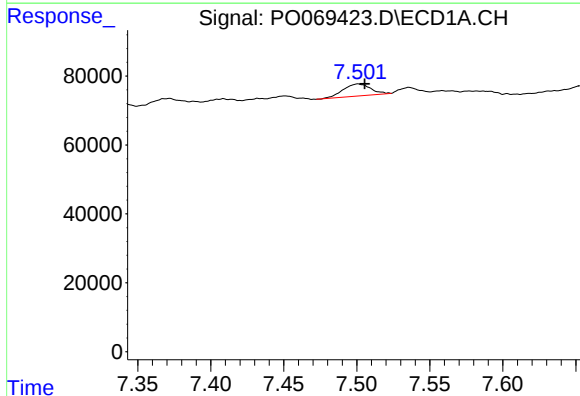


#29 AR-1254-4

R.T.: 7.501 min
Delta R.T.: -0.005 min
Response: 45794
Conc: 21.42 ng/ml

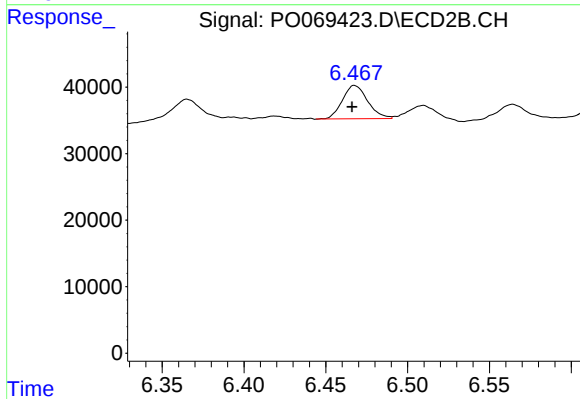

#29 AR-1254-4

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 53572
Conc: 23.60 ng/ml m

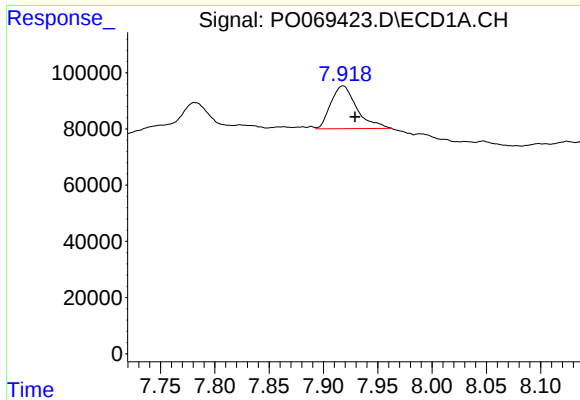


#30 AR-1254-5

R.T.: 7.918 min
Delta R.T.: -0.011 min
Response: 253454
Conc: 121.18 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-01

Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:17 AM

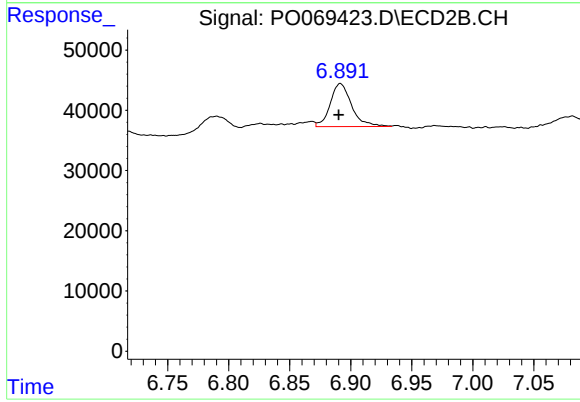

#30 AR-1254-5

R.T.: 6.891 min
Delta R.T.: 0.000 min
Response: 86911
Conc: 27.29 ng/ml m