

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070720\
 Data File : P0069425.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Jul 2020 11:37
 Operator : DD\AJ
 Sample : L3225-01RE 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-062220-SR-06

Manual Integrations
 APPROVED

Ankita
 7/8/2020 10:19:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 07 12:43:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Jun 29 12:05:30 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.563	174639	190171	5.903	4.941
2) SA Decachlor...	10.056	8.771	248774	438811	5.238m	8.061 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070720\
Data File : PO069425.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Jul 2020 11:37
Operator : DD\AJ
Sample : L3225-01RE 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-06


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 07 12:43:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061820.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jun 29 12:05:30 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

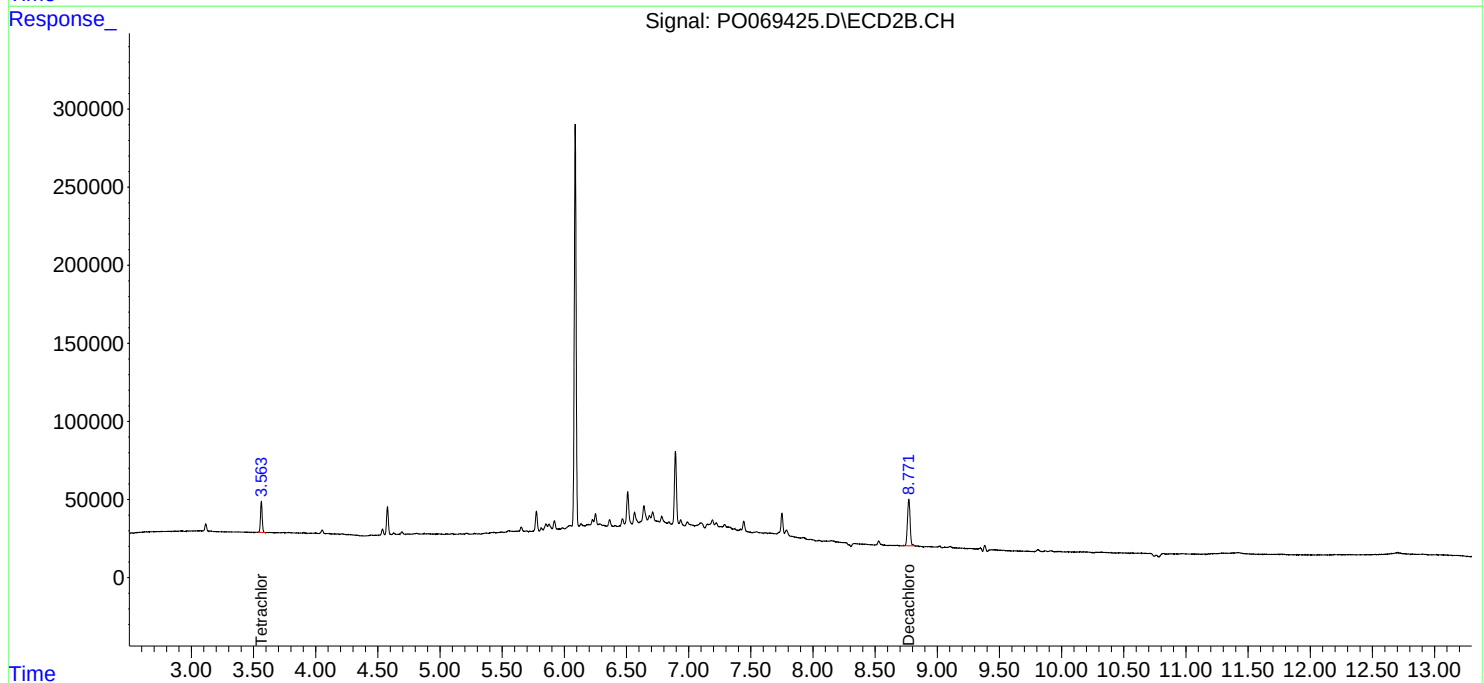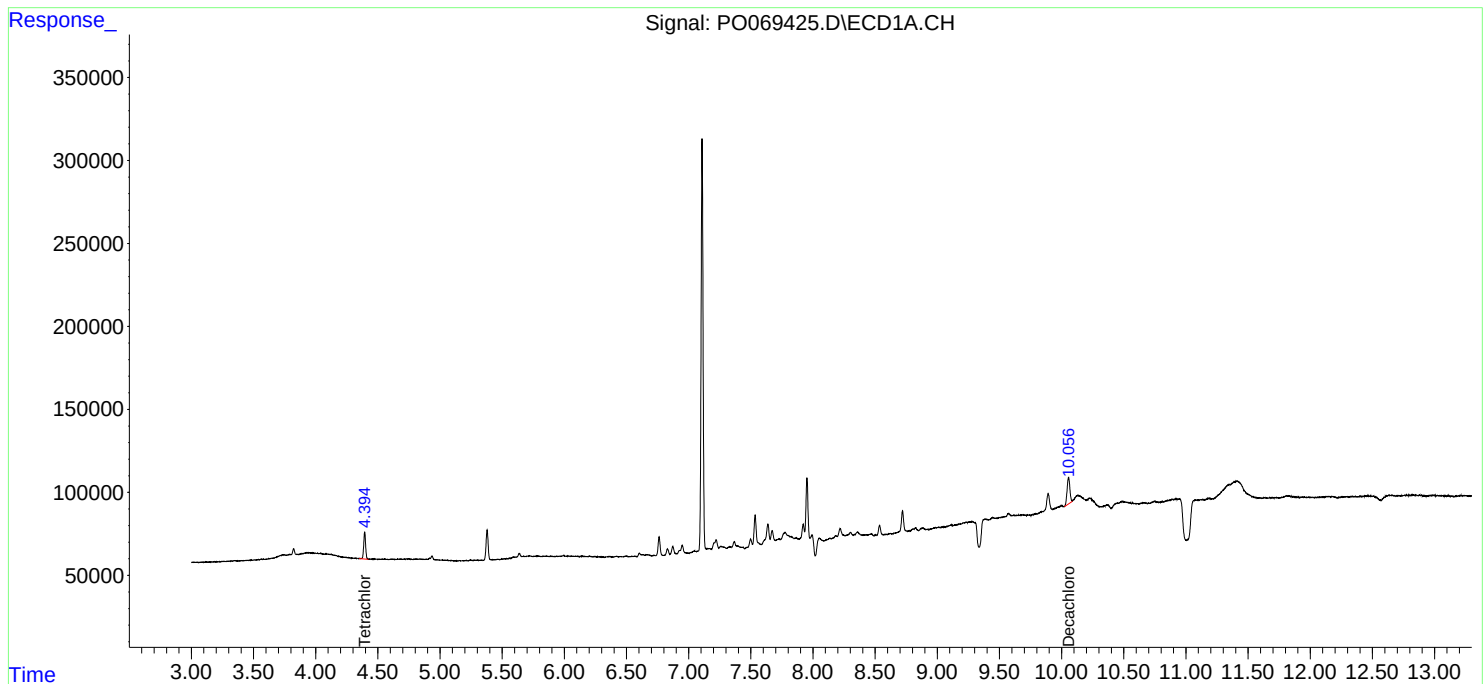

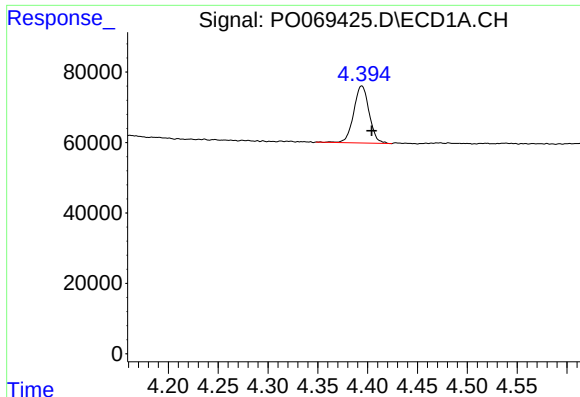


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: -0.010 min
Response: 174639
Conc: 5.90 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-062220-SR-06


Manual Integrations
APPROVED

Ankita
7/8/2020 10:19:21 AM

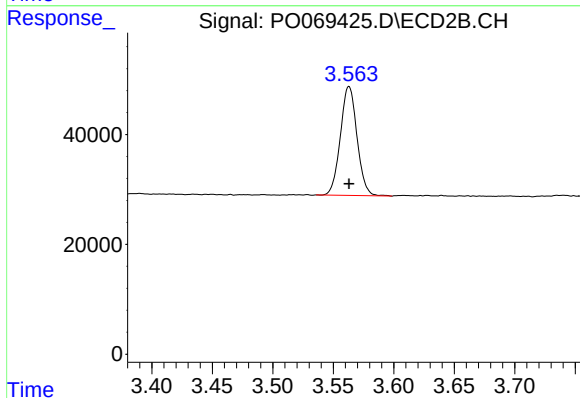


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.000 min
Response: 190171
Conc: 4.94 ng/ml

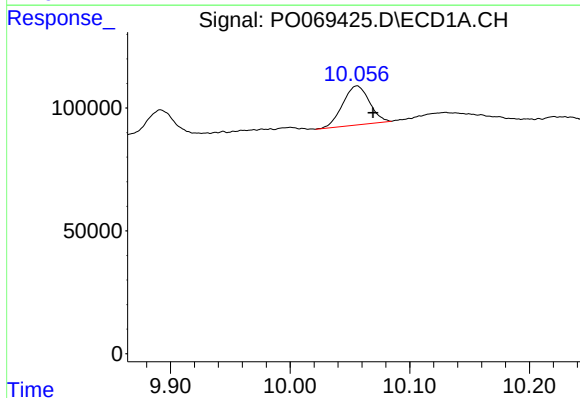

#2 Decachlorobiphenyl

R.T.: 10.056 min
Delta R.T.: -0.013 min
Response: 248774
Conc: 5.24 ng/ml m

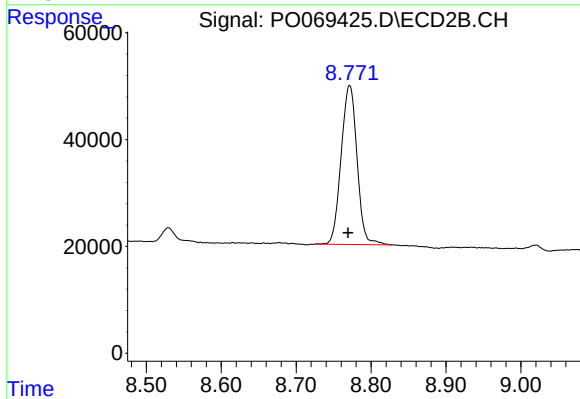

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: 0.002 min
Response: 438811
Conc: 8.06 ng/ml