

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070722\
 Data File : P0087826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2022 19:51
 Operator : YP/AJ
 Sample : N3605-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OE-2-070622

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2022
 Supervised By :Ankita Jodhani 07/08/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 03:16:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.607	51813316	20516964	20.018	20.851m
2) SA Decachlor...	10.299	8.611	46911312	14598189	22.966	18.008

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070722\
Data File : PO087826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2022 19:51
Operator : YP/AJ
Sample : N3605-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OE-2-070622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 03:16:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

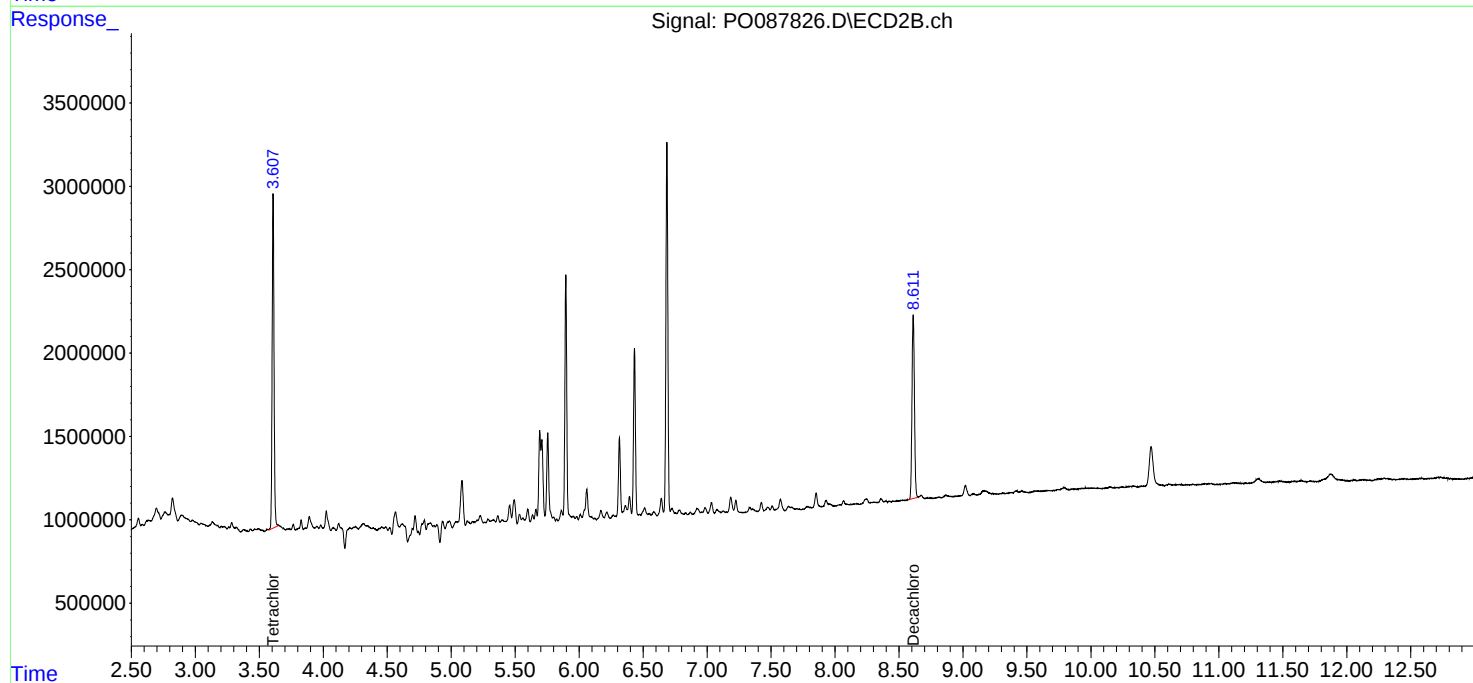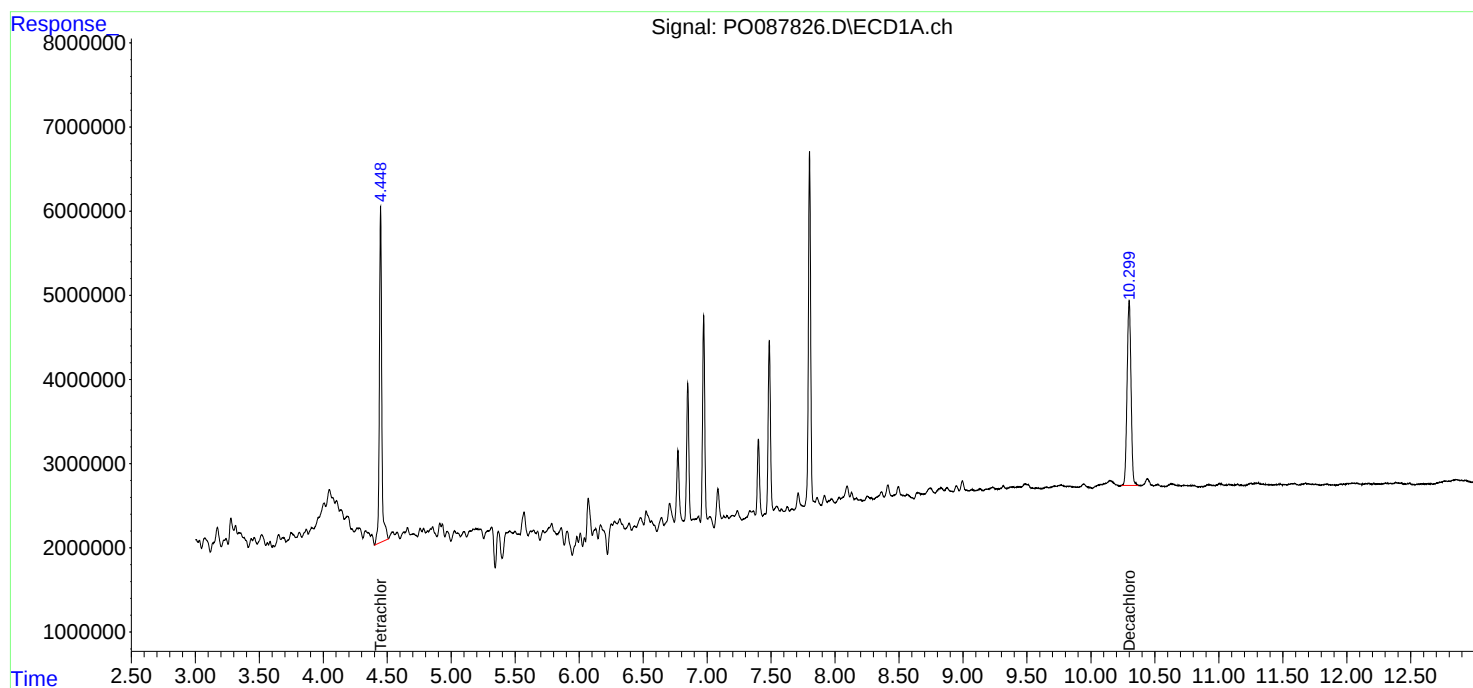

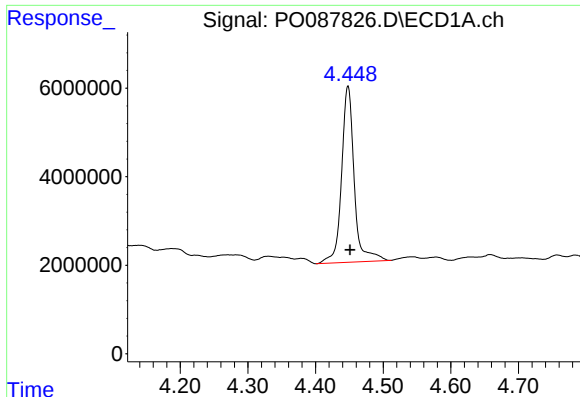


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 51813316
Conc: 20.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
OE-2-070622


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2022
Supervised By :Ankita Jodhani 07/08/2022

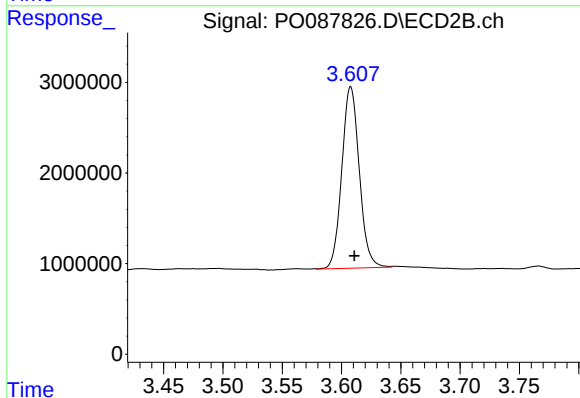


#1 Tetrachloro-m-xylene

R.T.: 3.607 min
Delta R.T.: -0.004 min
Response: 20516964
Conc: 20.85 ng/ml m

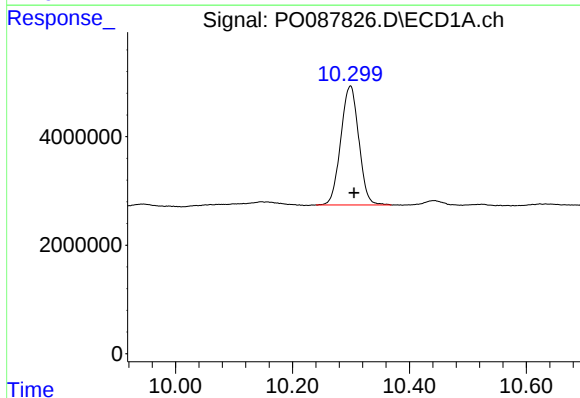

#2 Decachlorobiphenyl

R.T.: 10.299 min
Delta R.T.: -0.006 min
Response: 46911312
Conc: 22.97 ng/ml

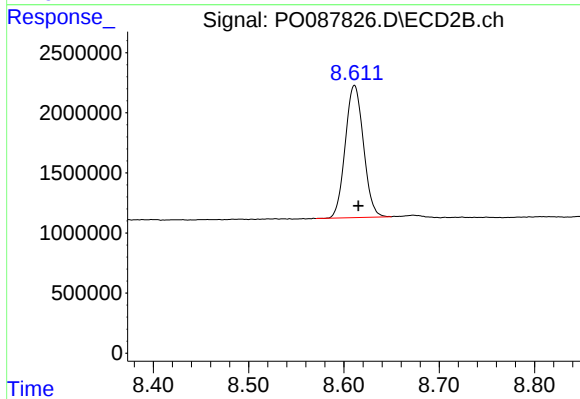

#2 Decachlorobiphenyl

R.T.: 8.611 min
Delta R.T.: -0.004 min
Response: 14598189
Conc: 18.01 ng/ml