

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070725\
 Data File : P0112047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 18:03
 Operator : YP/AJ
 Sample : Q2508-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-25-0105

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:55:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.675	3.669	64100263	59486598	11.130m	10.590m
2) SA Decachlor...	8.705	8.652	32164198	14970755	6.127	8.422m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070725\
Data File : PO112047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 18:03
Operator : YP/AJ
Sample : Q2508-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-25-0105


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 01:55:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

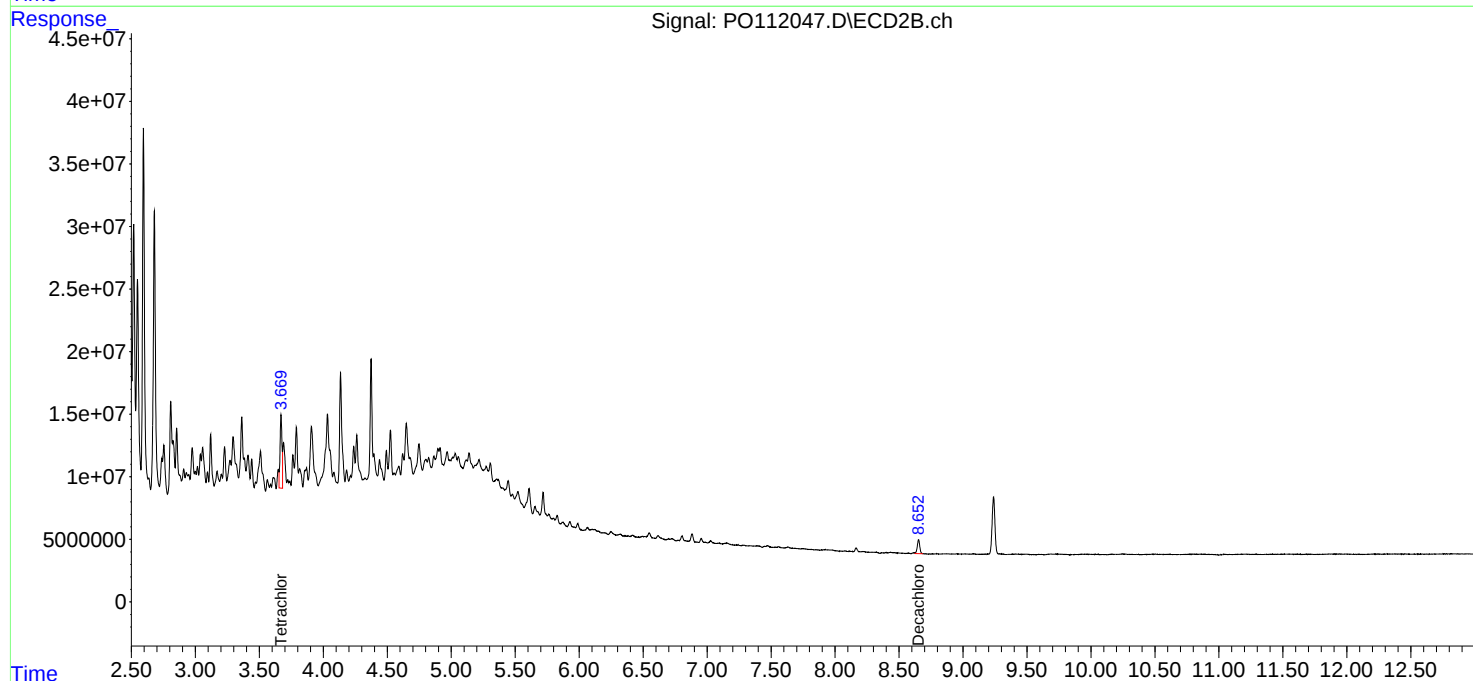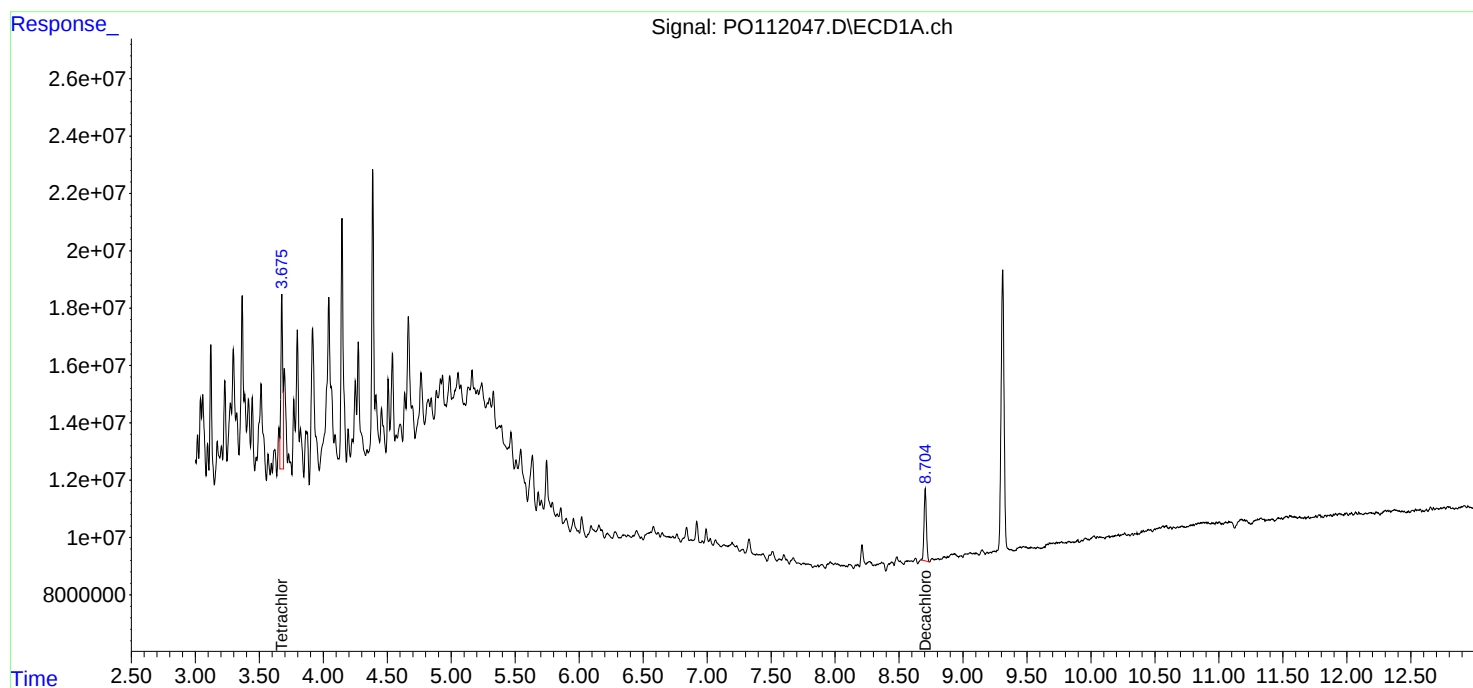

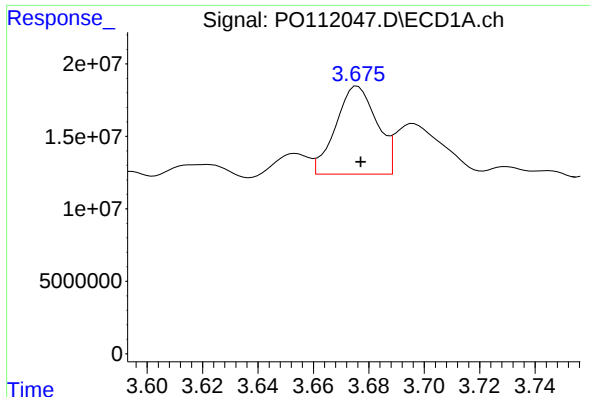


#1 Tetrachloro-m-xylene

R.T.: 3.675 min
Delta R.T.: -0.002 min
Response: 64100263
Conc: 11.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-25-0105


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

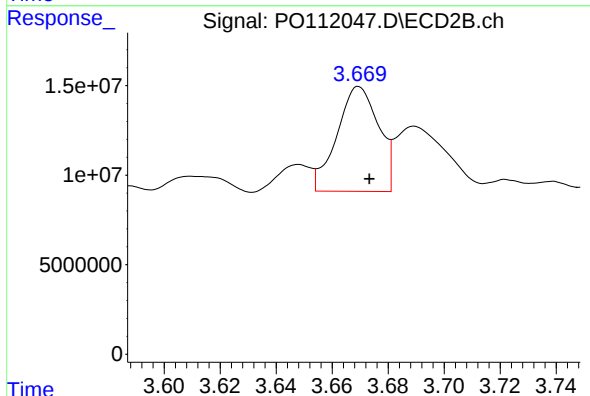


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: -0.004 min
Response: 59486598
Conc: 10.59 ng/ml m

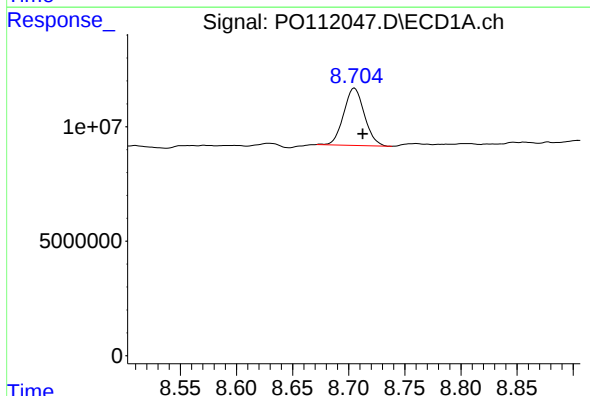

#2 Decachlorobiphenyl

R.T.: 8.705 min
Delta R.T.: -0.007 min
Response: 32164198
Conc: 6.13 ng/ml

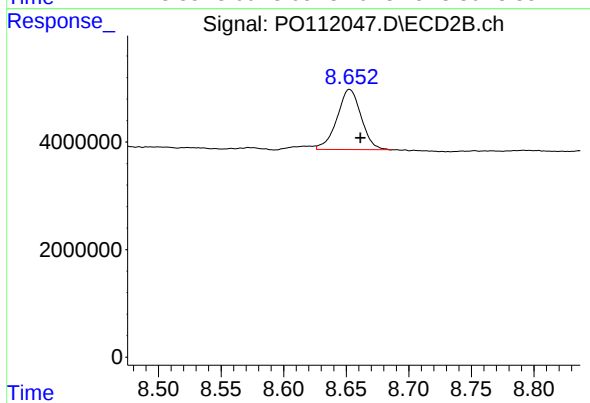

#2 Decachlorobiphenyl

R.T.: 8.652 min
Delta R.T.: -0.009 min
Response: 14970755
Conc: 8.42 ng/ml m