

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0070725\
 Data File : P0112051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 19:14
 Operator : YP/AJ
 Sample : Q2509-02 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 AUD-25-0112

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:56:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.674	3.670	10423485	10879673	1.810m	1.937m
2) SA Decachlor...	8.704	8.648	3405835	1526884	0.649m	0.859m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070725\
Data File : PO112051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 19:14
Operator : YP/AJ
Sample : Q2509-02 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-25-0112


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 01:56:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

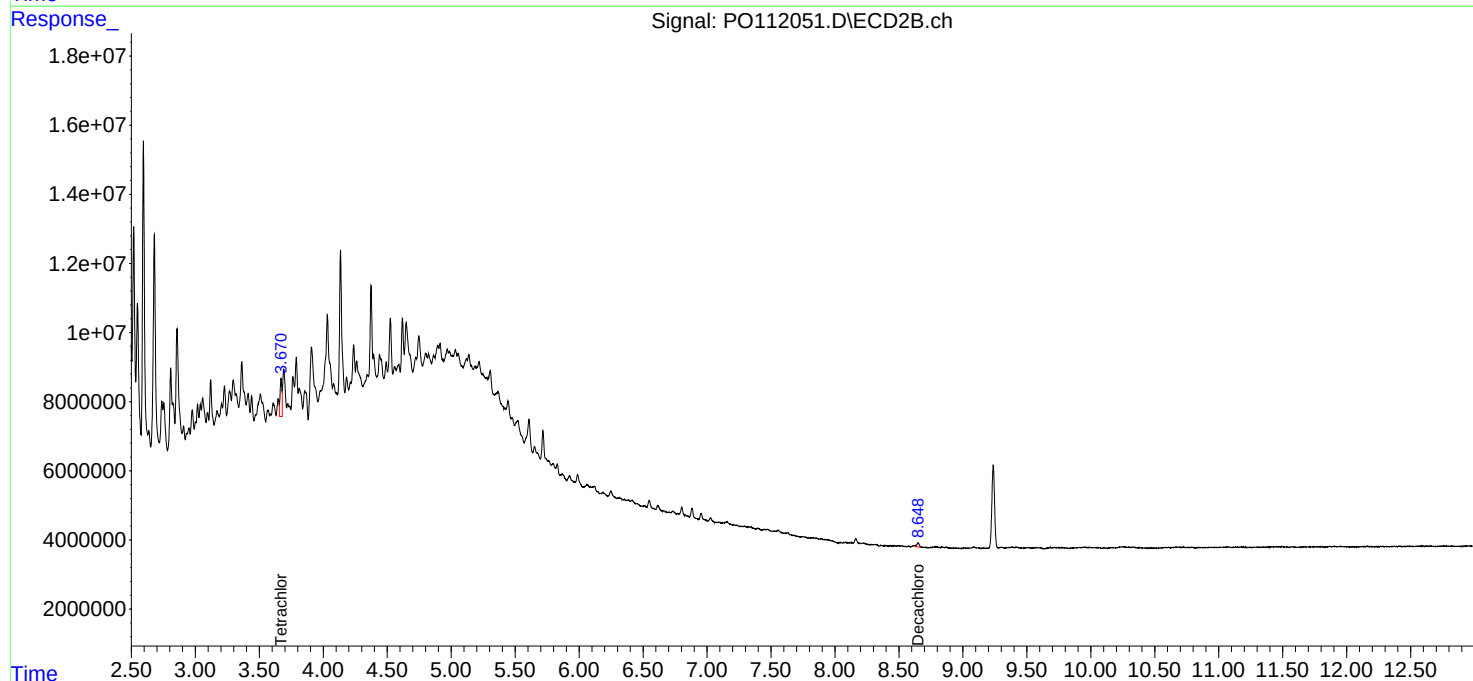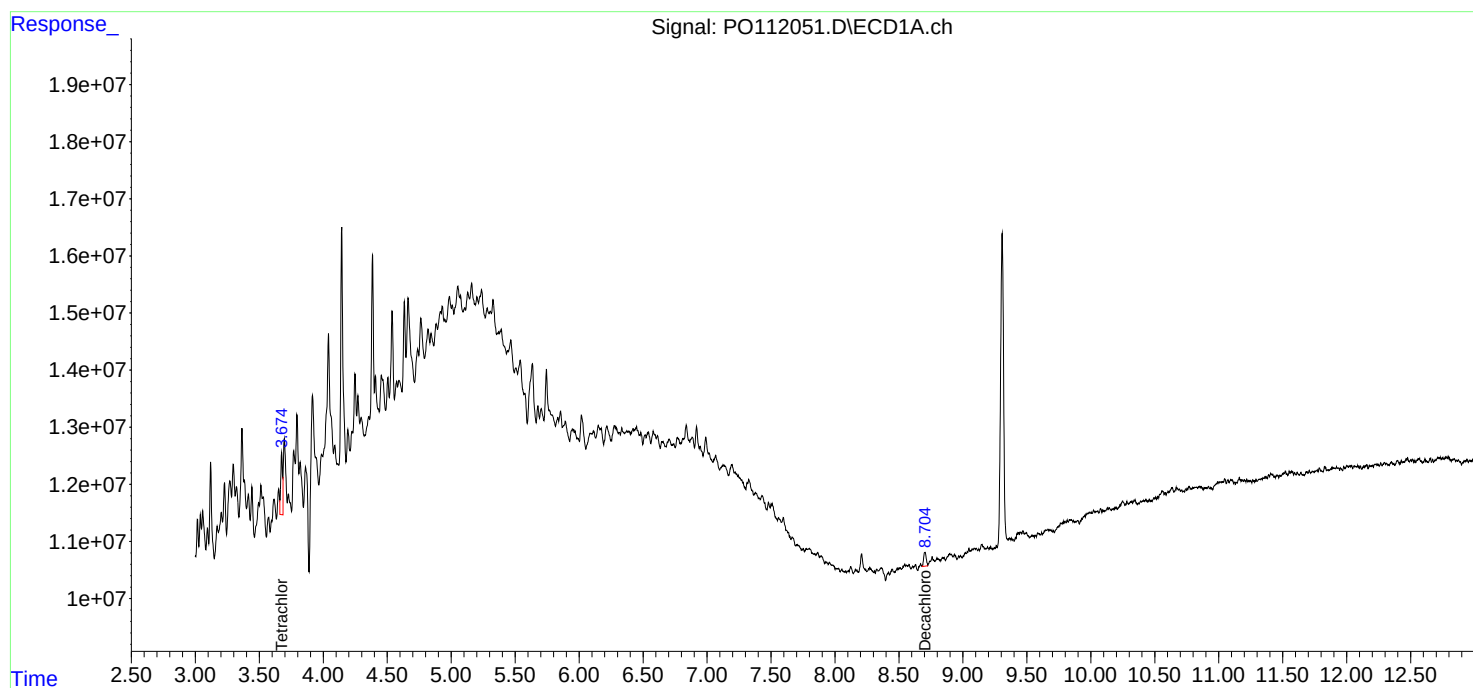

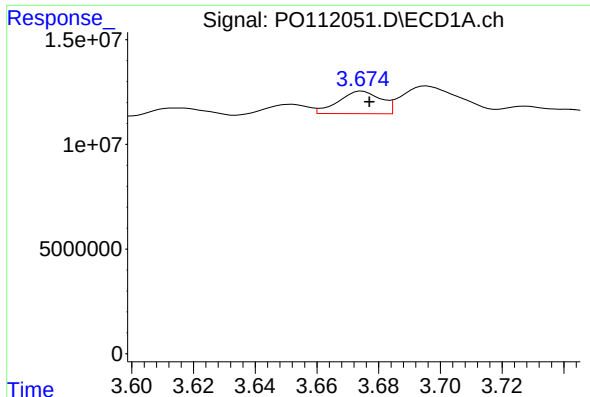


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 10423485
Conc: 1.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-25-0112


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

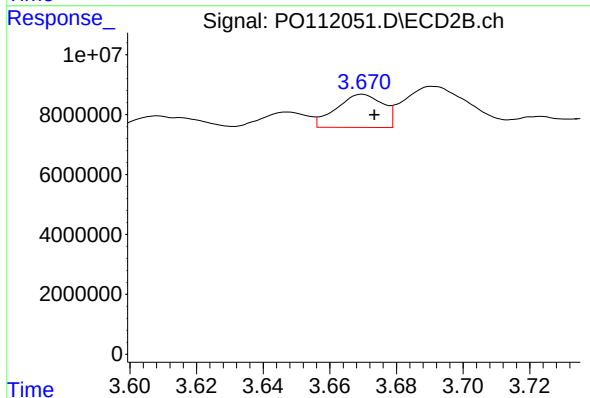


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: -0.004 min
Response: 10879673
Conc: 1.94 ng/ml m

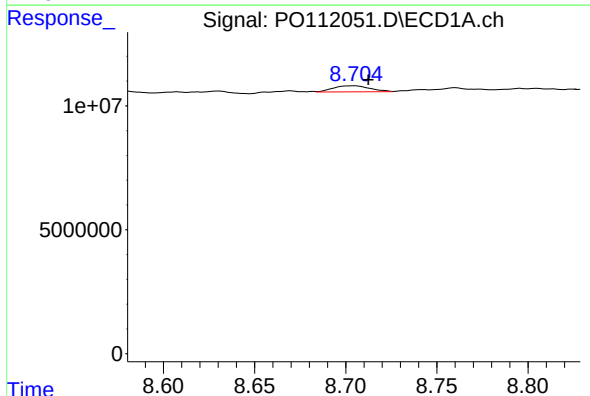

#2 Decachlorobiphenyl

R.T.: 8.704 min
Delta R.T.: -0.008 min
Response: 3405835
Conc: 0.65 ng/ml m

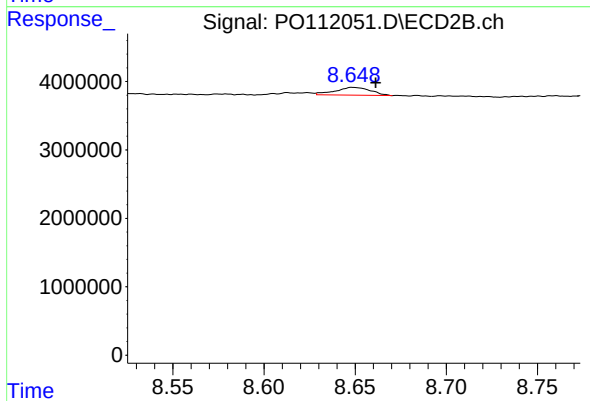

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.014 min
Response: 1526884
Conc: 0.86 ng/ml m