

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070725\
 Data File : P0112062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jul 2025 23:33
 Operator : YP/AJ
 Sample : Q2513-03
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HR-3-070325

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/08/2025
 Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 01:59:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0061125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jun 12 06:25:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.674	3.667	95771426	80766583	16.629	14.378m
2) SA Decachlor...	8.703	8.650	52909738	25156622	10.079m	14.152m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070725\
Data File : PO112062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jul 2025 23:33
Operator : YP/AJ
Sample : Q2513-03
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HR-3-070325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 01:59:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO061125.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jun 12 06:25:26 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

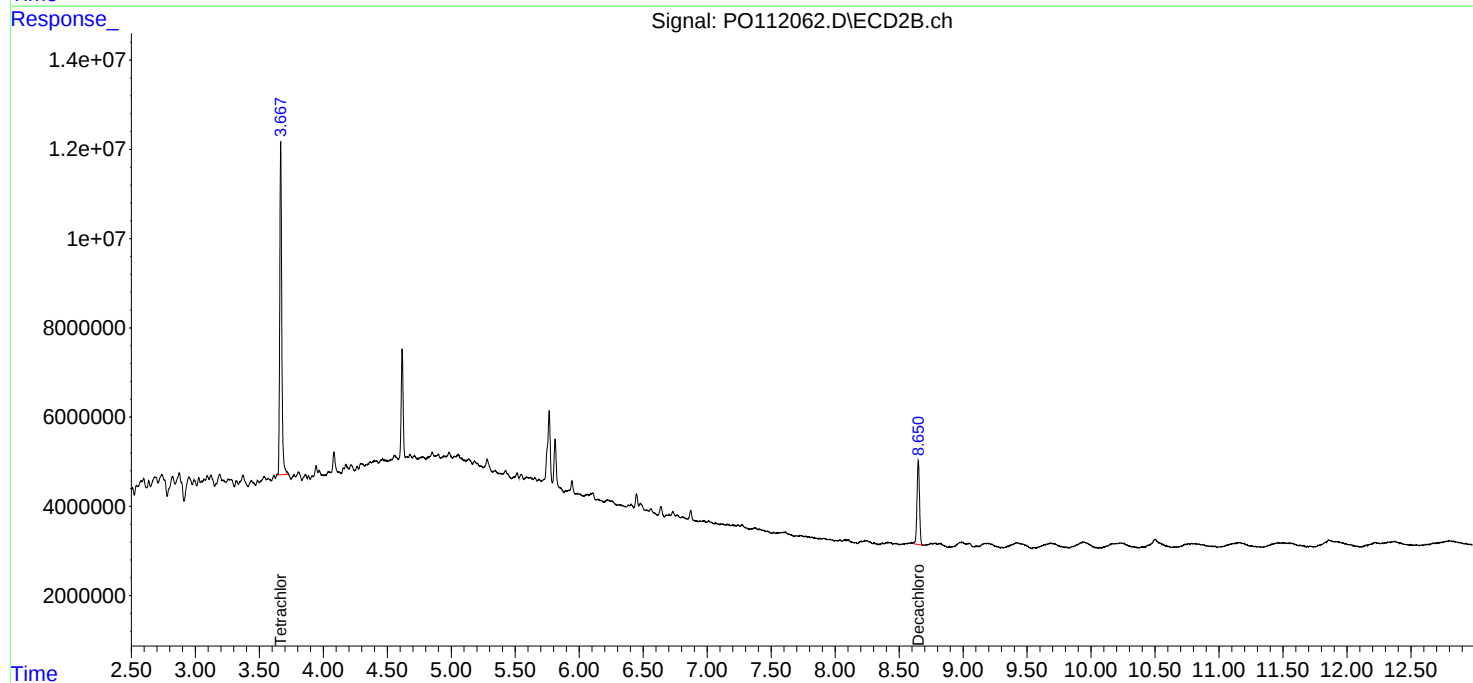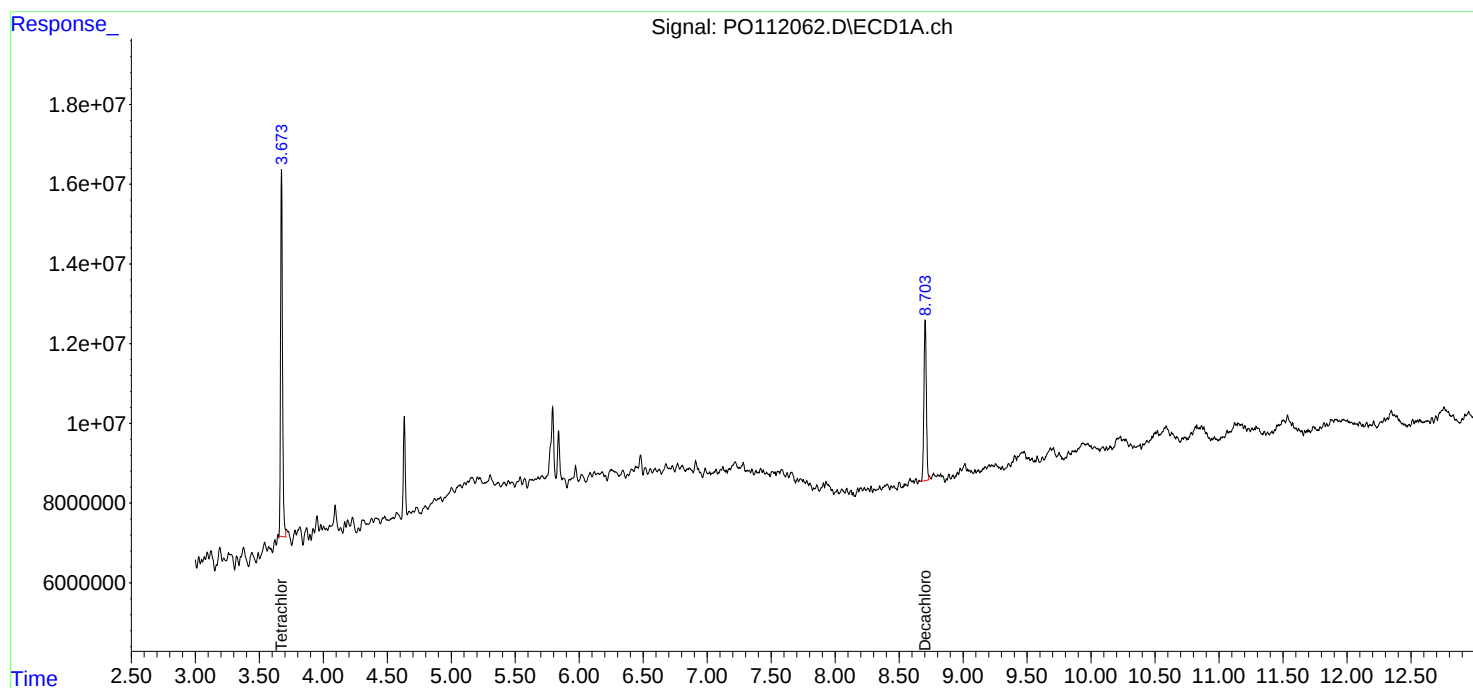

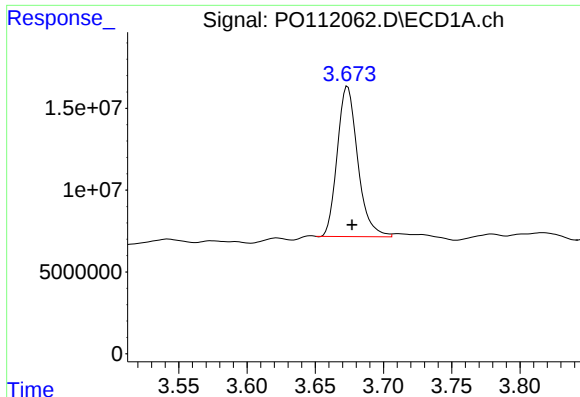


#1 Tetrachloro-m-xylene

R.T.: 3.674 min
Delta R.T.: -0.003 min
Response: 95771426
Conc: 16.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
HR-3-070325


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/08/2025
Supervised By :mohammad ahmed 07/09/2025

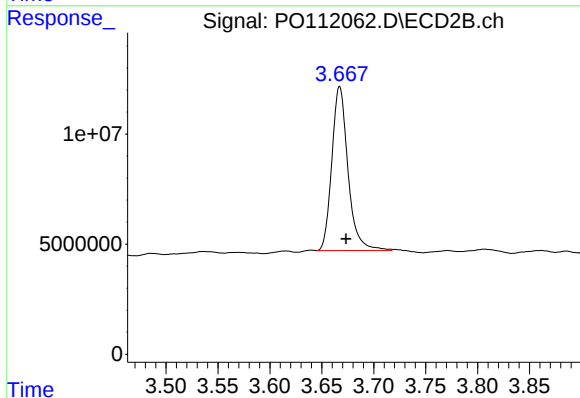


#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: -0.007 min
Response: 80766583
Conc: 14.38 ng/ml m

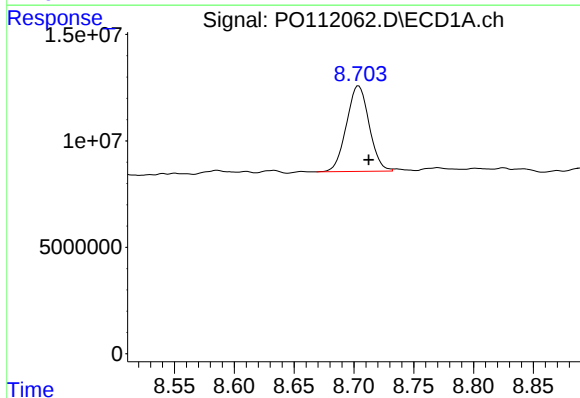

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: -0.009 min
Response: 52909738
Conc: 10.08 ng/ml m

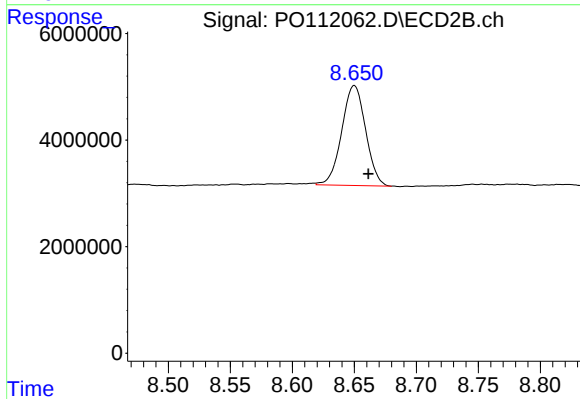

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: -0.012 min
Response: 25156622
Conc: 14.15 ng/ml m