

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070820\
 Data File : P0069449.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Jul 2020 14:31
 Operator : DD\AJ
 Sample : L3183-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-02-070720

Manual Integrations
 APPROVED

Ankita
 7/9/2020 10:20:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 08 17:25:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.391	3.563	886752	939649	23.751m	23.611
2) SA Decachlor...	10.055	8.774	1157171	977667	19.233m	17.226

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070820\
Data File : P0069449.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Jul 2020 14:31
Operator : DD\AJ
Sample : L3183-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-02-070720


Manual Integrations
APPROVED

Ankita
7/9/2020 10:20:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 08 17:25:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

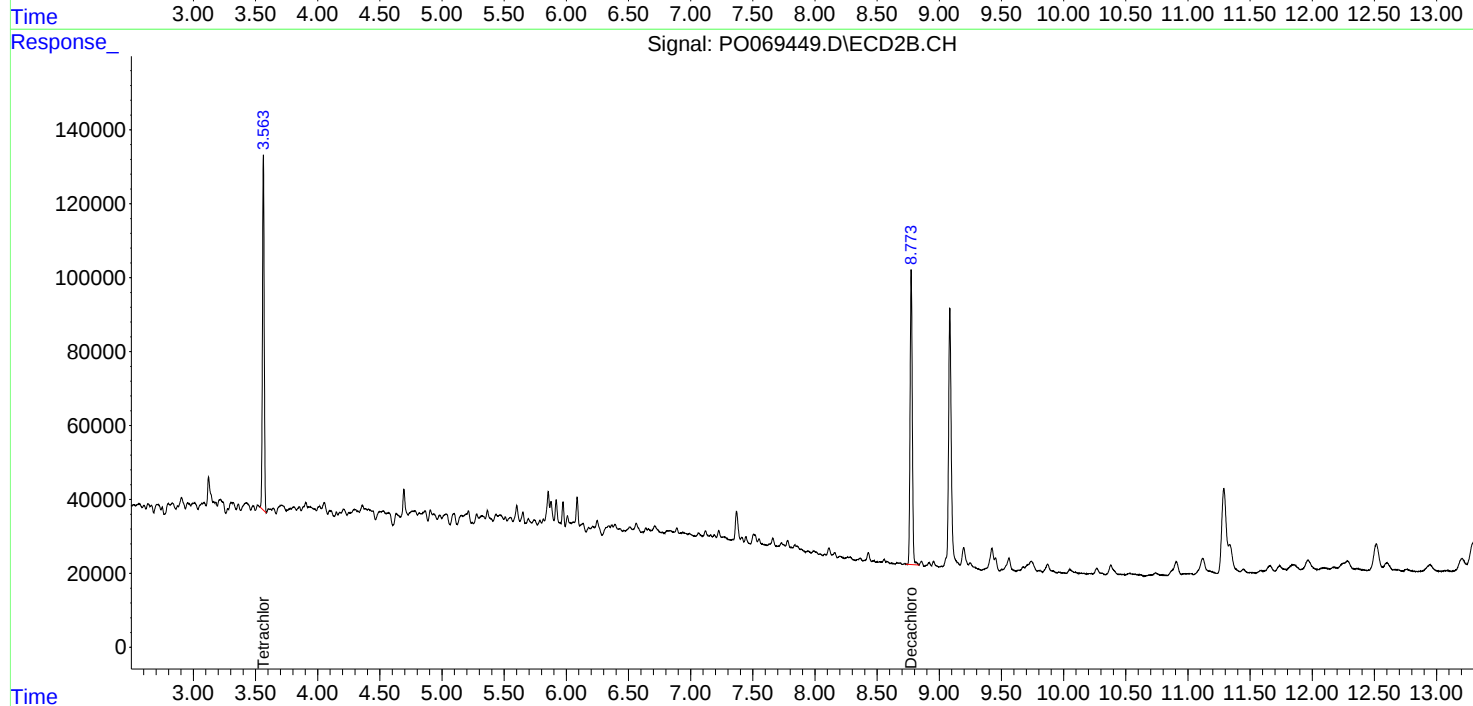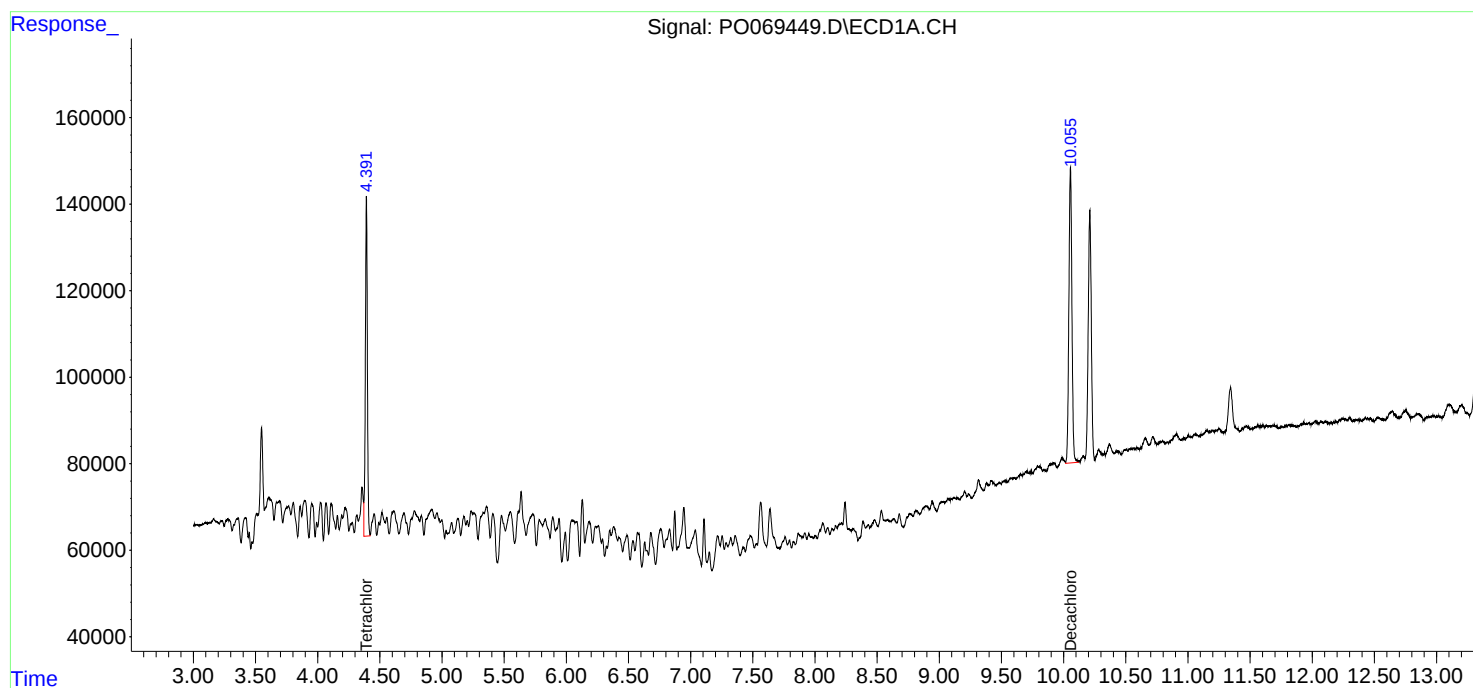

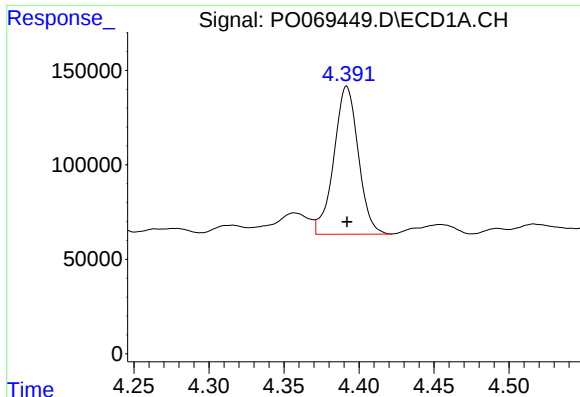

#1 Tetrachloro-m-xylene

R.T.: 4.391 min

Delta R.T.: 0.000 min


Response: 886752

Conc: 23.75 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-02-070720

Manual Integrations
APPROVED

Ankita
7/9/2020 10:20:40 AM

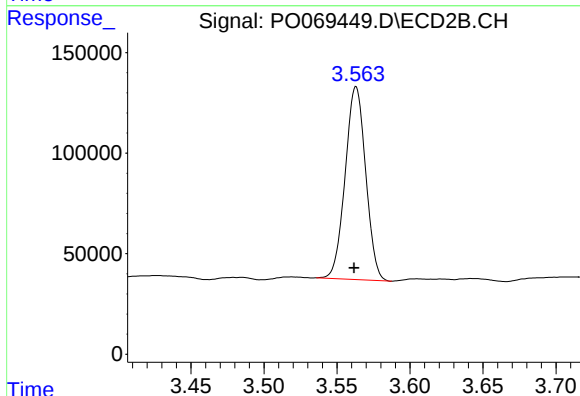


#1 Tetrachloro-m-xylene

R.T.: 3.563 min

Delta R.T.: 0.001 min

Response: 939649

Conc: 23.61 ng/ml

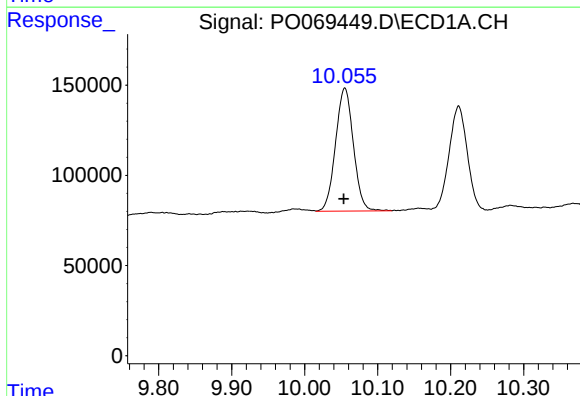


#2 Decachlorobiphenyl

R.T.: 10.055 min

Delta R.T.: 0.001 min

Response: 1157171

Conc: 19.23 ng/ml m

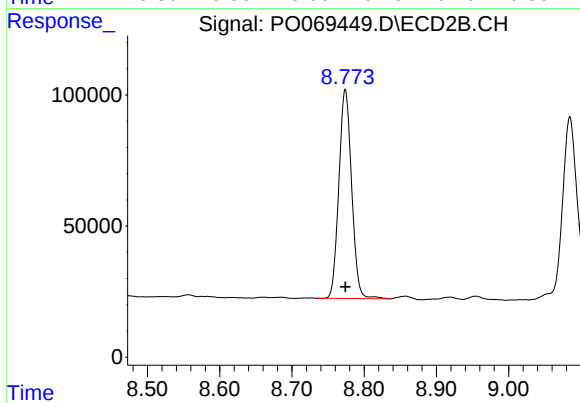

#2 Decachlorobiphenyl

R.T.: 8.774 min

Delta R.T.: 0.000 min

Response: 977667

Conc: 17.23 ng/ml