

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070822\
 Data File : P0087890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2022 00:04
 Operator : YP/AJ
 Sample : N3619-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31654

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/11/2022
 Supervised By :Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 06:37:03 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.448	3.609	42376462	19157884	16.372m	19.470
2) SA Decachlor...	10.295	8.608	27281884	9604369	13.356	11.848m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070822\
Data File : PO087890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2022 00:04
Operator : YP/AJ
Sample : N3619-04
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
31654


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 06:37:03 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

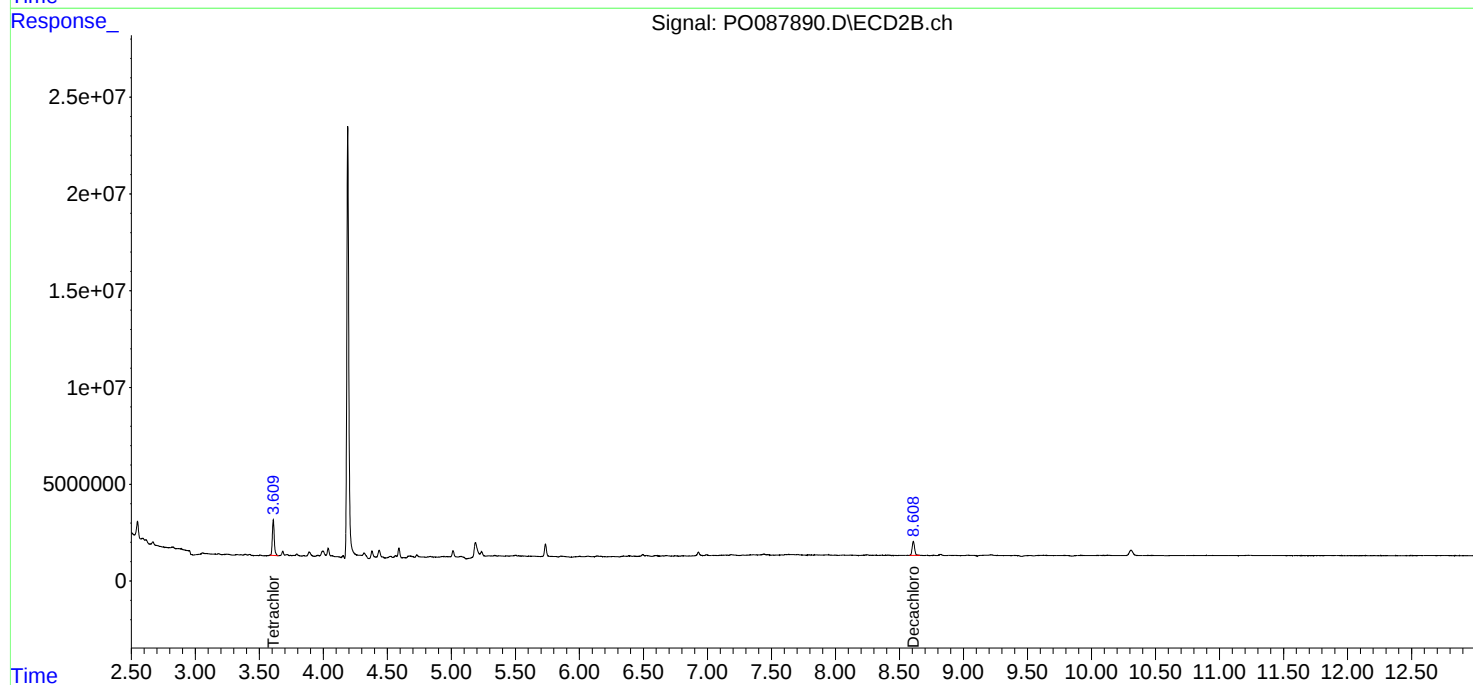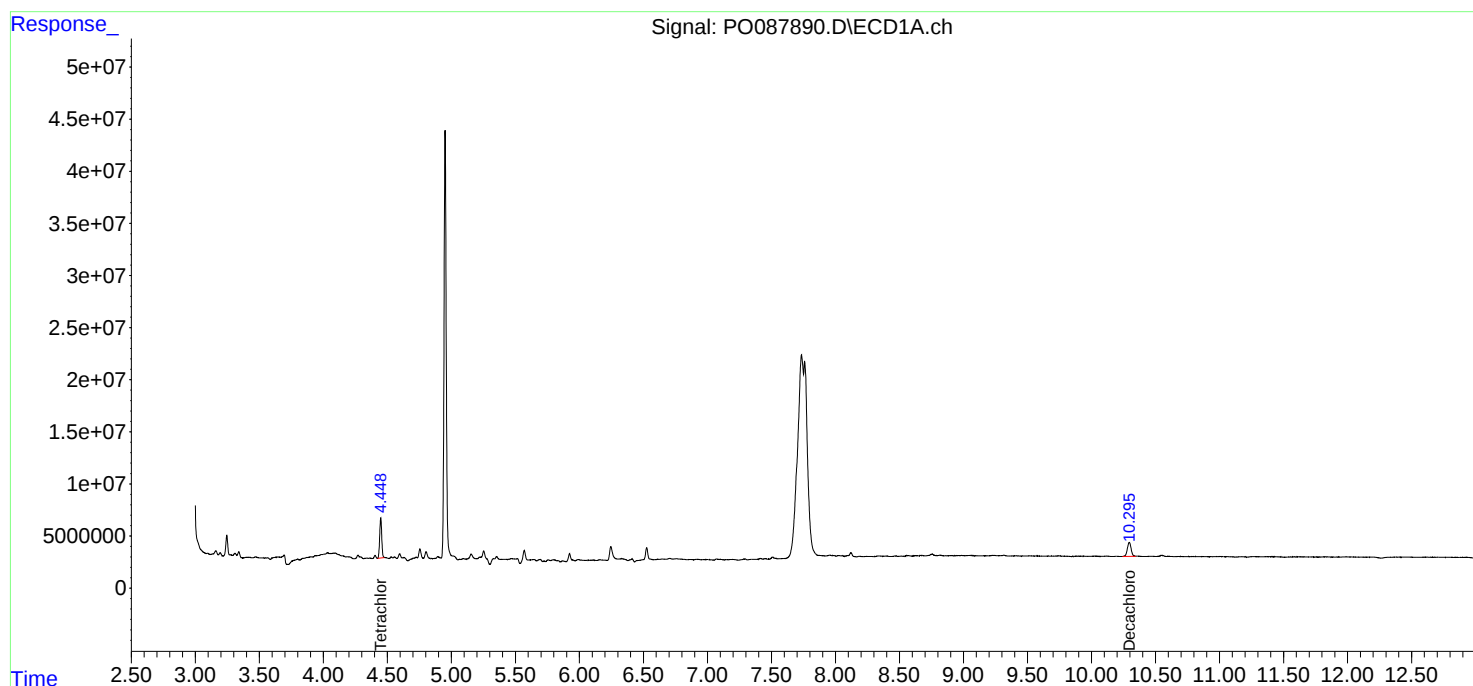

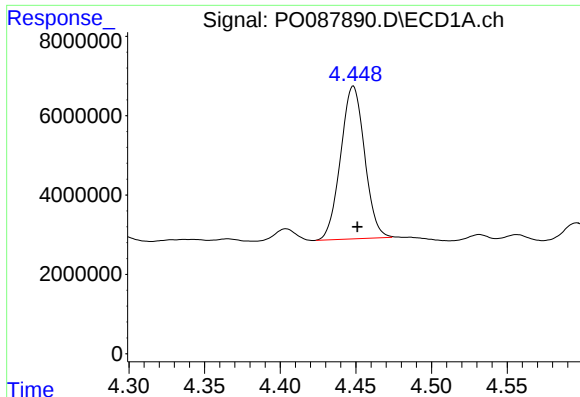


#1 Tetrachloro-m-xylene

R.T.: 4.448 min
Delta R.T.: -0.003 min
Response: 42376462
Conc: 16.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
31654


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2022
Supervised By :Ankita Jodhani 07/11/2022

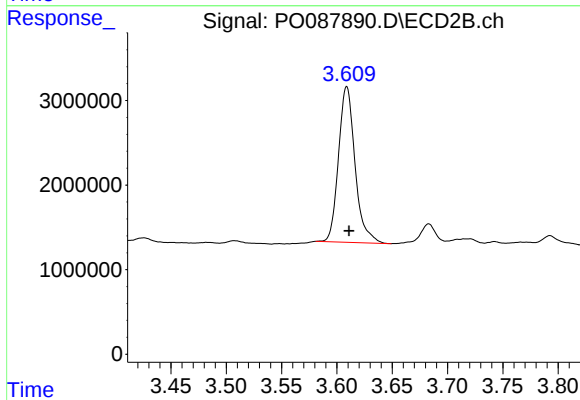


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.002 min
Response: 19157884
Conc: 19.47 ng/ml

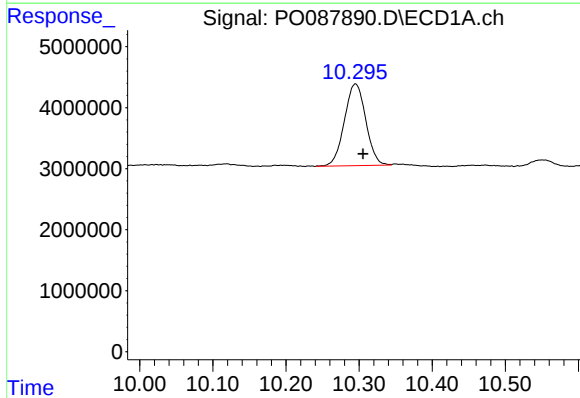

#2 Decachlorobiphenyl

R.T.: 10.295 min
Delta R.T.: -0.010 min
Response: 27281884
Conc: 13.36 ng/ml

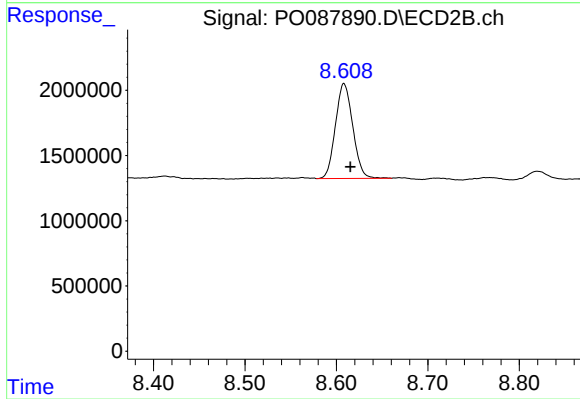

#2 Decachlorobiphenyl

R.T.: 8.608 min
Delta R.T.: -0.008 min
Response: 9604369
Conc: 11.85 ng/ml m