

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070822\
 Data File : P0087891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Jul 2022 00:21
 Operator : YP/AJ
 Sample : N3621-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-047-IDWGW-20220706

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 09 06:37:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0062722.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Jun 28 02:46:21 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.447	3.608	43937476	17800408	16.975	18.090
2) SA Decachlor...	10.293	8.607	15215757	5316036	7.449	6.558

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070822\
Data File : PO087891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Jul 2022 00:21
Operator : YP/AJ
Sample : N3621-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-047-IDWGW-20220706

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 09 06:37:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO062722.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Jun 28 02:46:21 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

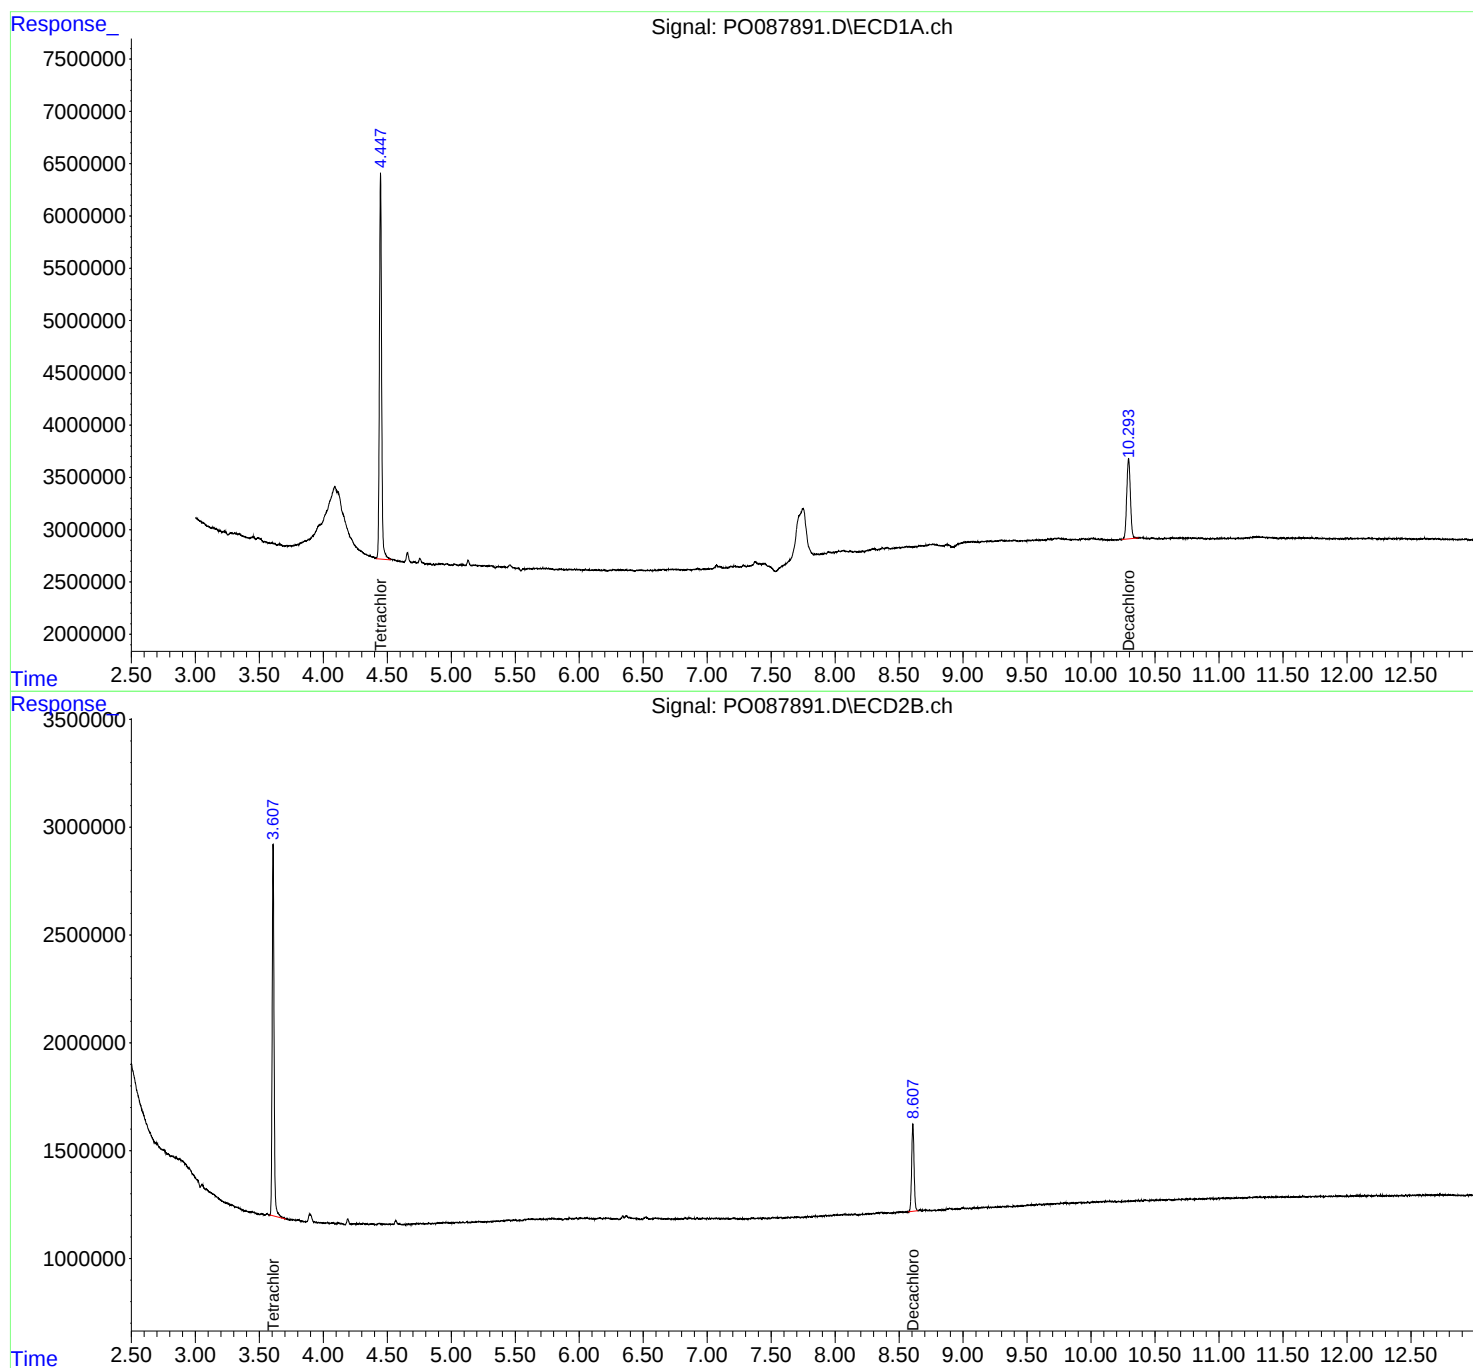


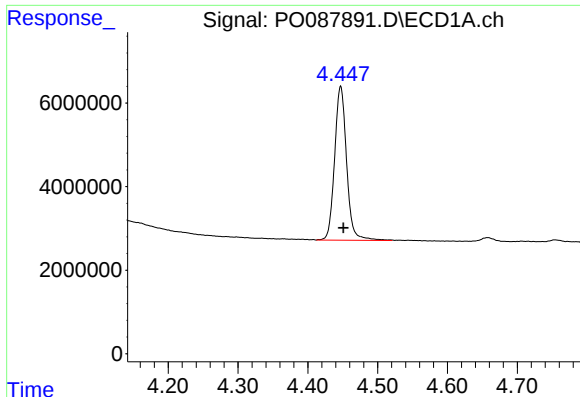

#1 Tetrachloro-m-xylene


R.T.: 4.447 min
Delta R.T.: -0.004 min
Response: 43937476
Conc: 16.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-047-IDWGW-20220706

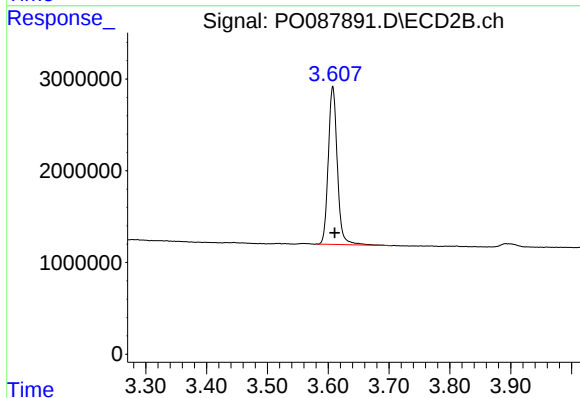


#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.003 min
Response: 17800408
Conc: 18.09 ng/ml

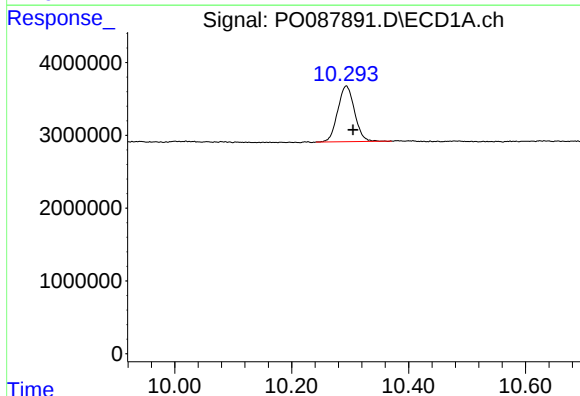

#2 Decachlorobiphenyl

R.T.: 10.293 min
Delta R.T.: -0.012 min
Response: 15215757
Conc: 7.45 ng/ml

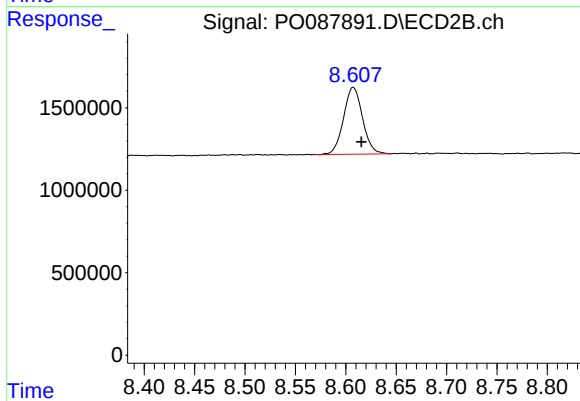

#2 Decachlorobiphenyl

R.T.: 8.607 min
Delta R.T.: -0.008 min
Response: 5316036
Conc: 6.56 ng/ml