

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070920\
 Data File : P0069493.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2020 22:51
 Operator : DD\AJ
 Sample : L3263-03DL 5X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-01-SDL

Manual Integrations
 APPROVED

Ankita
 7/10/2020 12:33:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 02:28:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.565	176029	195423	4.715	4.911
2) SA Decachlor...	10.051	8.776	329554	392621	5.477m	6.918 #
Target Compounds						
26) L6 AR-1254-1	6.596	5.655	239348	401424	120.240m	154.211 #
27) L6 AR-1254-2	6.826	5.817	500042	541408	155.765	234.520 #
28) L6 AR-1254-3	7.202	6.228	661779	884668	188.429	235.566 #
29) L6 AR-1254-4	7.498	6.469	573940	556918	191.769	220.375
30) L6 AR-1254-5	7.921	6.893	874461	1104178	290.635	307.660

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070920\
Data File : PO069493.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2020 22:51
Operator : DD\AJ
Sample : L3263-03DL 5X
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-01-SDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 02:28:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

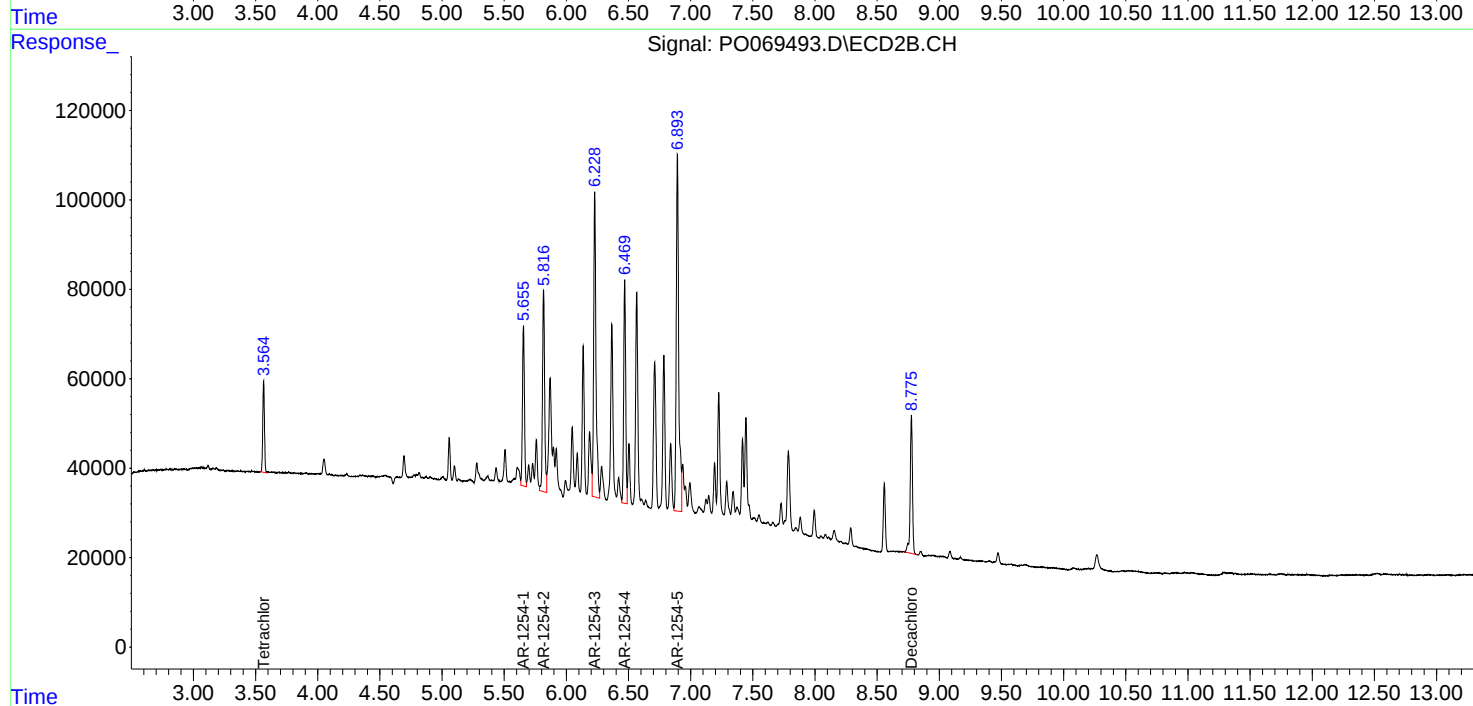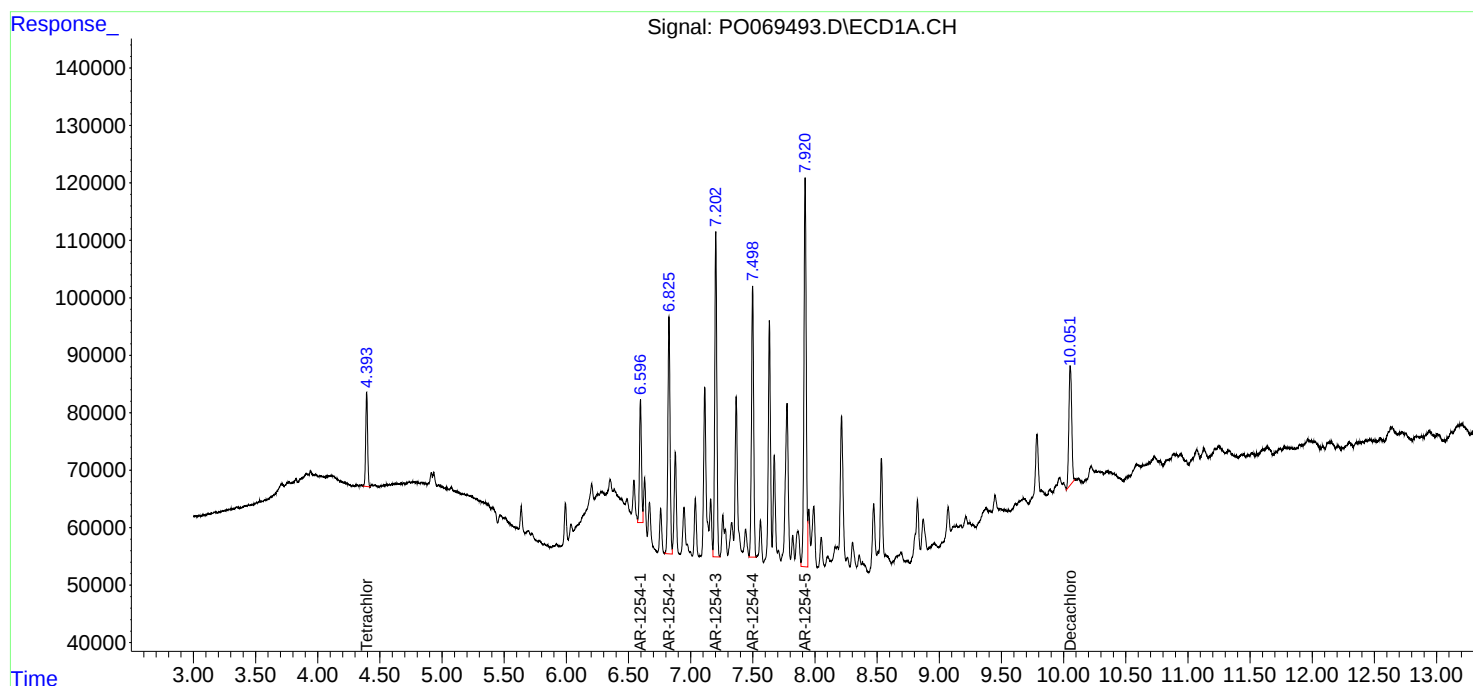

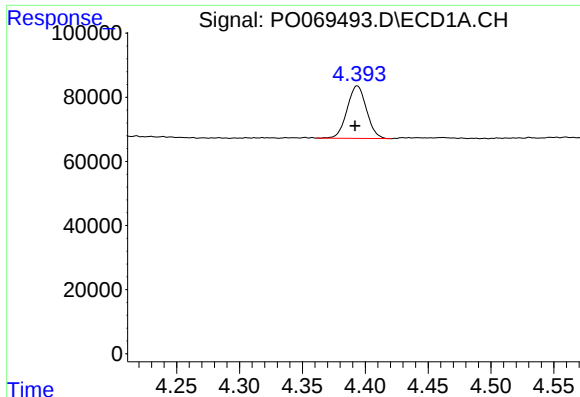


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: 0.002 min
Response: 176029
Conc: 4.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-SDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:55 PM

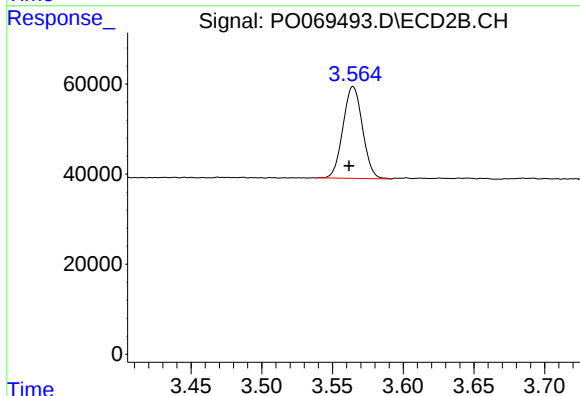


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.003 min
Response: 195423
Conc: 4.91 ng/ml

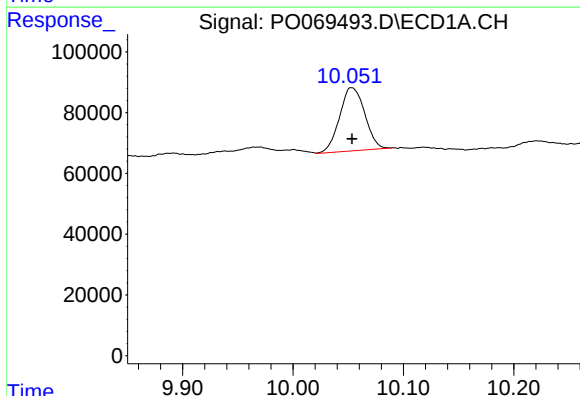


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: -0.002 min
Response: 329554
Conc: 5.48 ng/ml m

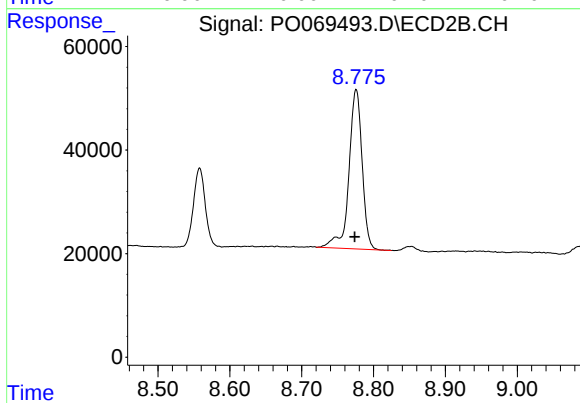

#2 Decachlorobiphenyl

R.T.: 8.776 min
Delta R.T.: 0.002 min
Response: 392621
Conc: 6.92 ng/ml

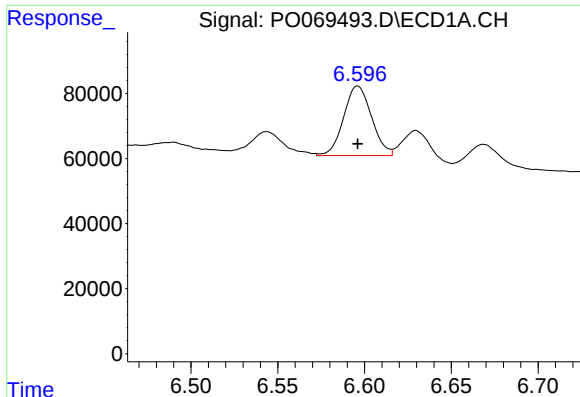


#26 AR-1254-1

R.T.: 6.596 min
Delta R.T.: 0.000 min
Response: 239348
Conc: 120.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-01-SDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:55 PM

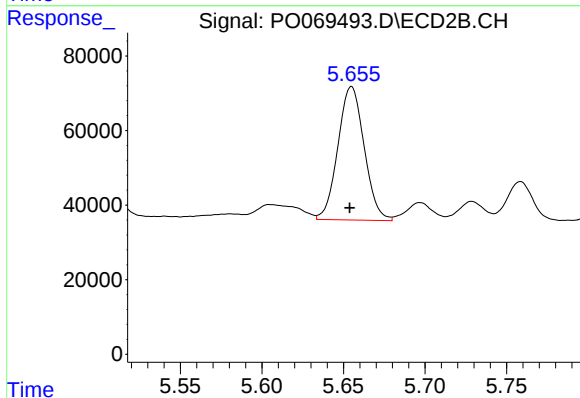


#26 AR-1254-1

R.T.: 5.655 min
Delta R.T.: 0.001 min
Response: 401424
Conc: 154.21 ng/ml

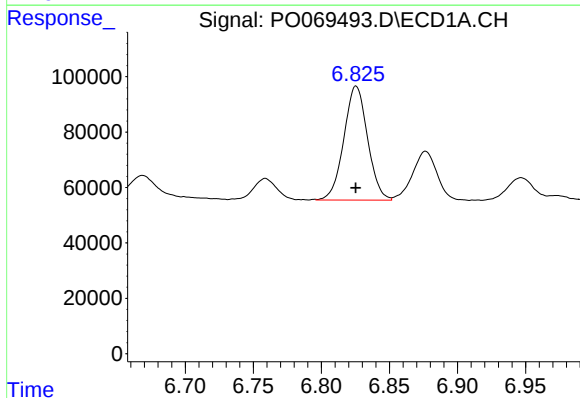


#27 AR-1254-2

R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 500042
Conc: 155.76 ng/ml

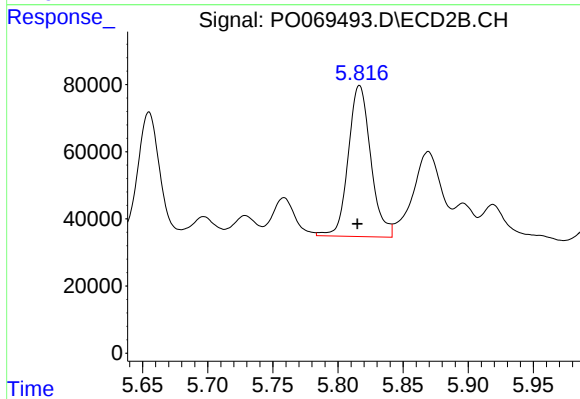

#27 AR-1254-2

R.T.: 5.817 min
Delta R.T.: 0.002 min
Response: 541408
Conc: 234.52 ng/ml

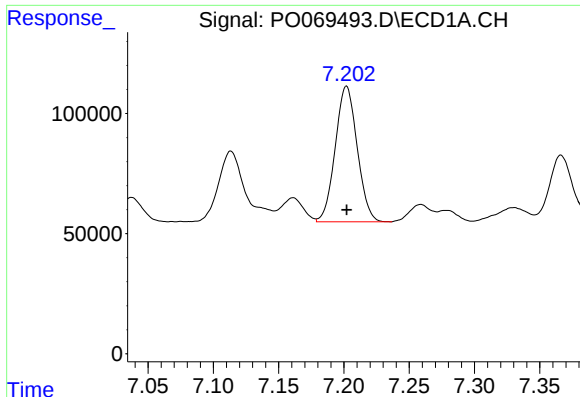


#28 AR-1254-3

R.T.: 7.202 min
Delta R.T.: 0.000 min
Response: 661779
Conc: 188.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-SDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:55 PM

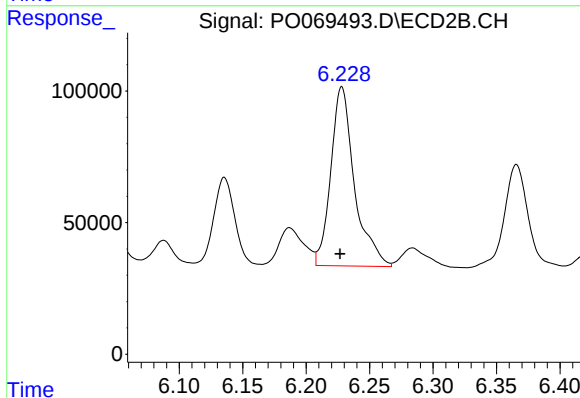


#28 AR-1254-3

R.T.: 6.228 min
Delta R.T.: 0.002 min
Response: 884668
Conc: 235.57 ng/ml

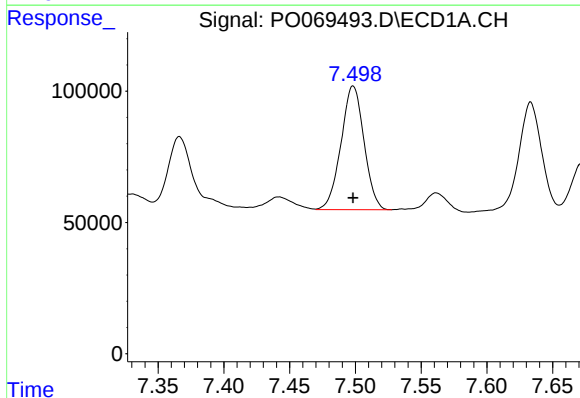


#29 AR-1254-4

R.T.: 7.498 min
Delta R.T.: 0.000 min
Response: 573940
Conc: 191.77 ng/ml

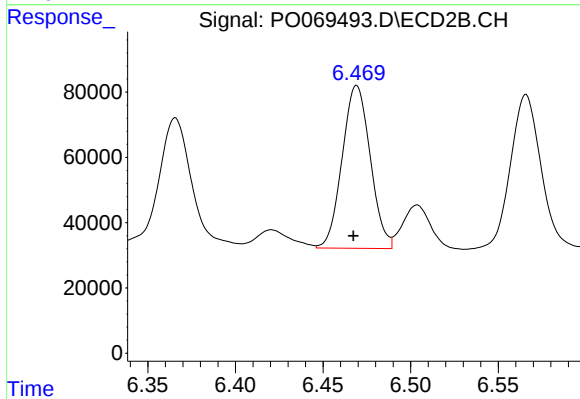

#29 AR-1254-4

R.T.: 6.469 min
Delta R.T.: 0.002 min
Response: 556918
Conc: 220.38 ng/ml

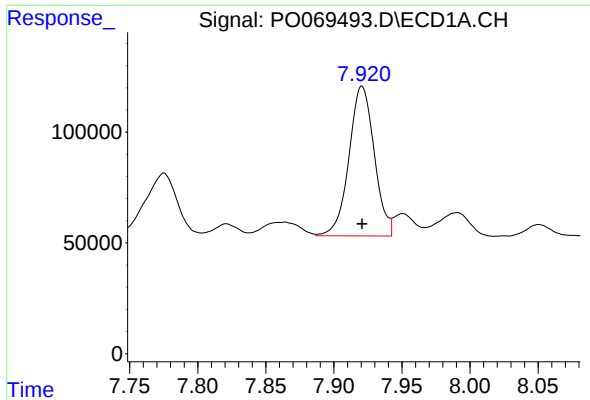


#30 AR-1254-5

R.T.: 7.921 min
Delta R.T.: 0.000 min
Response: 874461
Conc: 290.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-01-SDL

Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:55 PM

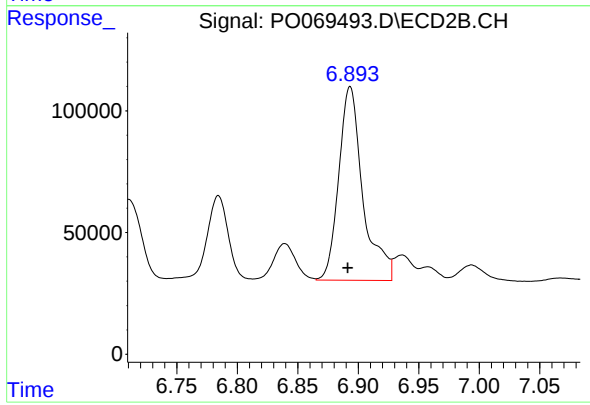

#30 AR-1254-5

R.T.: 6.893 min
Delta R.T.: 0.002 min
Response: 1104178
Conc: 307.66 ng/ml