

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070920\
 Data File : P0069494.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2020 23:08
 Operator : DD\AJ
 Sample : L3263-04DL 5X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S5-05-BDL

Manual Integrations
 APPROVED

Ankita
 7/10/2020 12:33:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 02:29:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.565	170993	185136	4.580	4.652
2) SA Decachlor...	10.055	8.775	223890	250610	3.721	4.416
Target Compounds						
26) L6 AR-1254-1	6.598	5.656	568289	731252	285.489m	280.917
27) L6 AR-1254-2	6.826	5.817	1050448	891455	327.218	386.150
28) L6 AR-1254-3	7.203	6.230	1150630	1508989	327.620	401.807
29) L6 AR-1254-4	7.499	6.470	1110035	1022073	370.893	404.440
30) L6 AR-1254-5	7.922	6.894	1623178	1965304	539.478	547.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070920\
Data File : P0069494.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2020 23:08
Operator : DD\AJ
Sample : L3263-04DL 5X
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S5-05-BDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 02:29:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

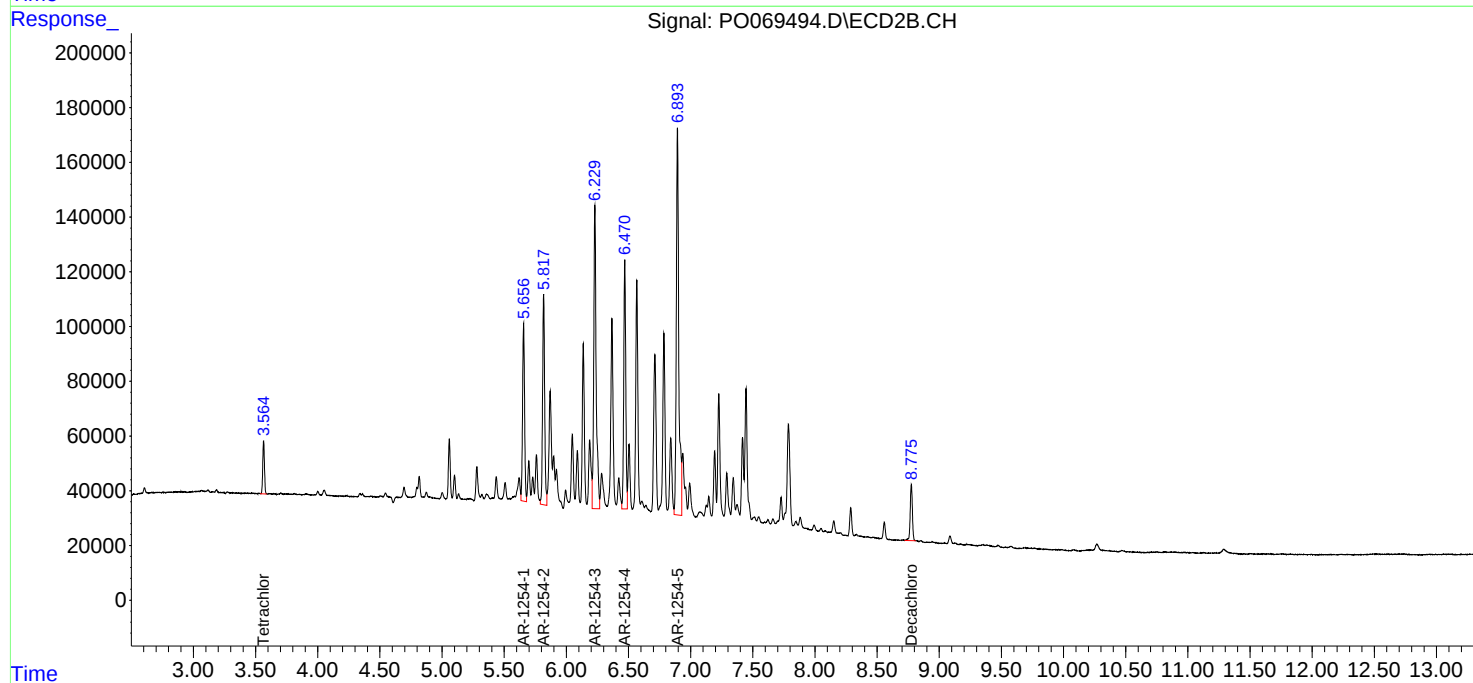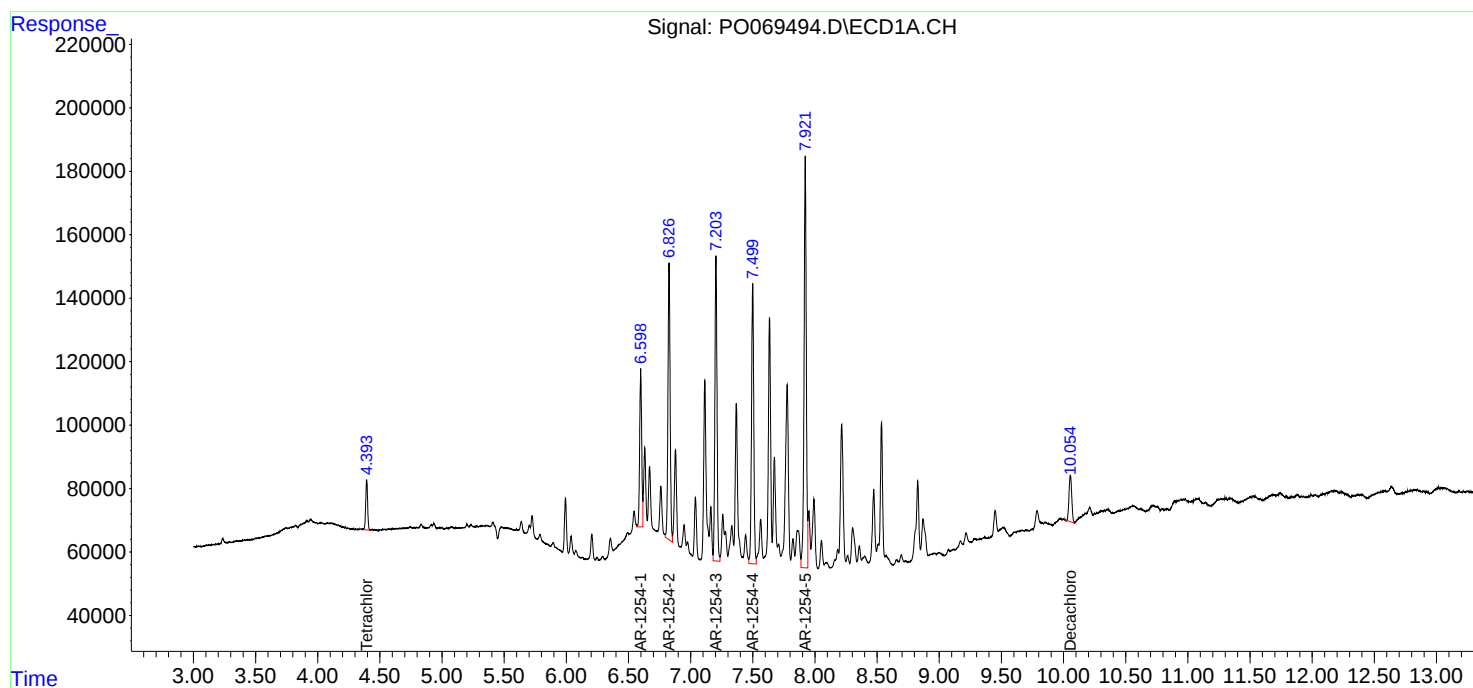

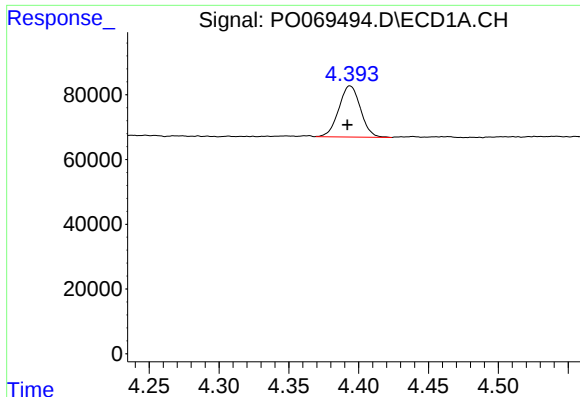


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: 0.002 min
Response: 170993
Conc: 4.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-BDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:57 PM

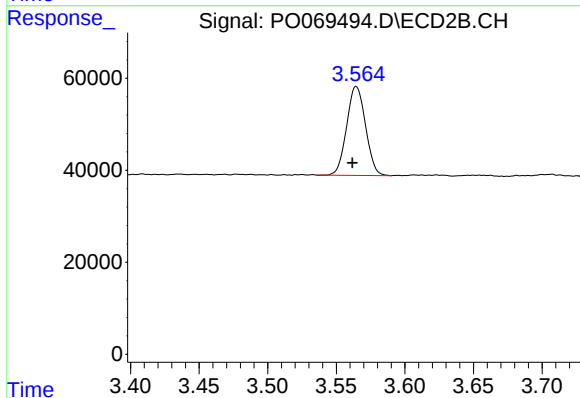


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: 0.003 min
Response: 185136
Conc: 4.65 ng/ml

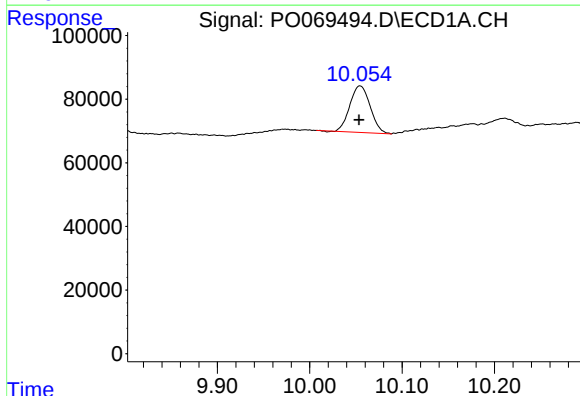


#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.001 min
Response: 223890
Conc: 3.72 ng/ml

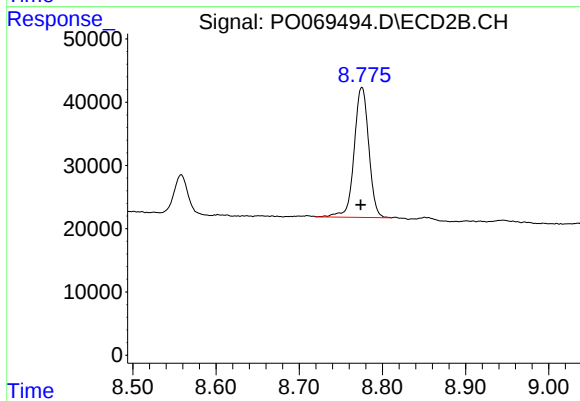

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: 0.001 min
Response: 250610
Conc: 4.42 ng/ml

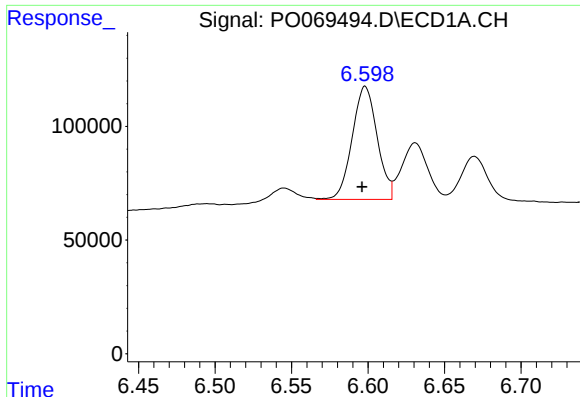


#26 AR-1254-1

R.T.: 6.598 min
Delta R.T.: 0.002 min
Response: 568289
Conc: 285.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S5-05-BDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:57 PM

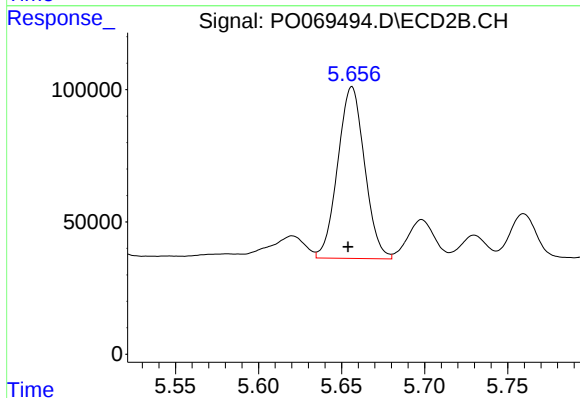


#26 AR-1254-1

R.T.: 5.656 min
Delta R.T.: 0.002 min
Response: 731252
Conc: 280.92 ng/ml

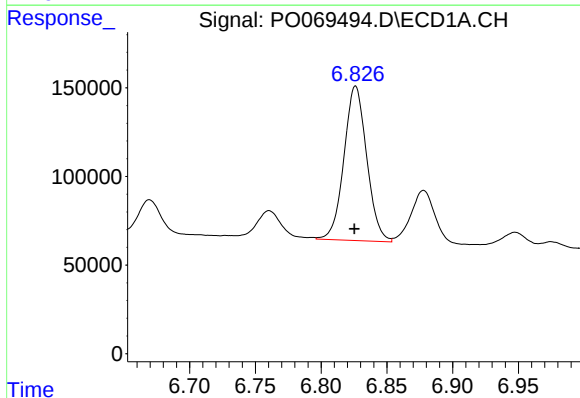


#27 AR-1254-2

R.T.: 6.826 min
Delta R.T.: 0.000 min
Response: 1050448
Conc: 327.22 ng/ml

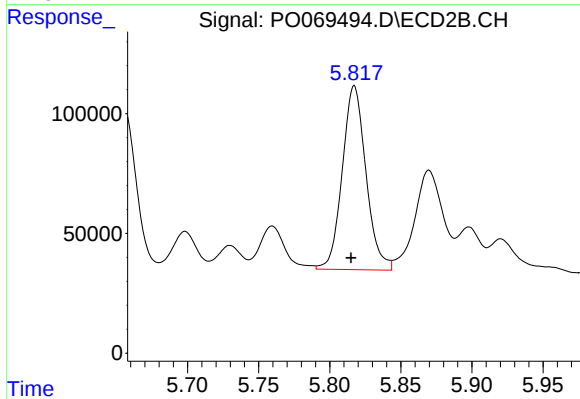

#27 AR-1254-2

R.T.: 5.817 min
Delta R.T.: 0.002 min
Response: 891455
Conc: 386.15 ng/ml

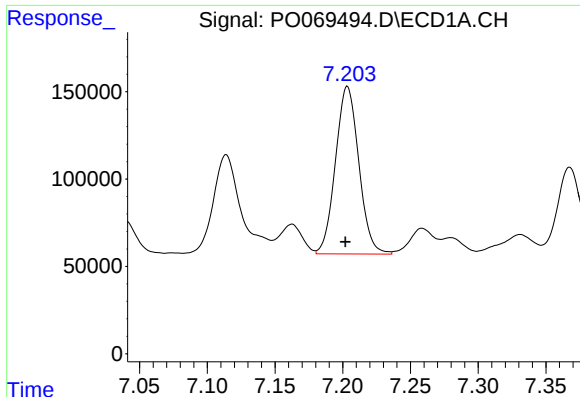


#28 AR-1254-3

R.T.: 7.203 min
Delta R.T.: 0.001 min
Response: 1150630
Conc: 327.62 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-BDL


Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:57 PM

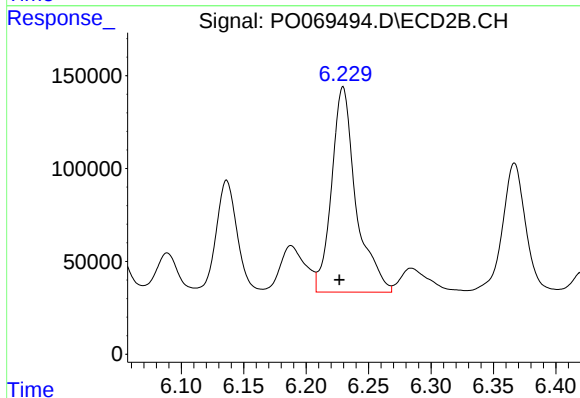


#28 AR-1254-3

R.T.: 6.230 min
Delta R.T.: 0.003 min
Response: 1508989
Conc: 401.81 ng/ml

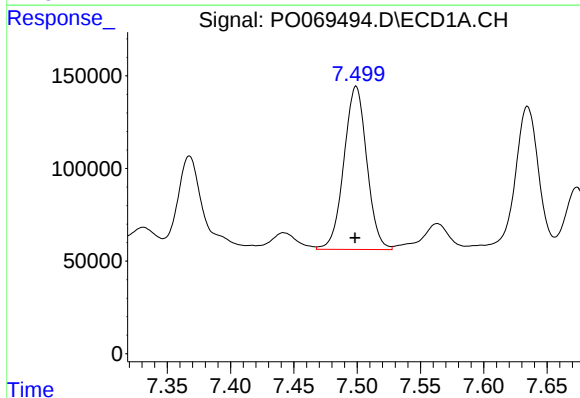


#29 AR-1254-4

R.T.: 7.499 min
Delta R.T.: 0.000 min
Response: 1110035
Conc: 370.89 ng/ml

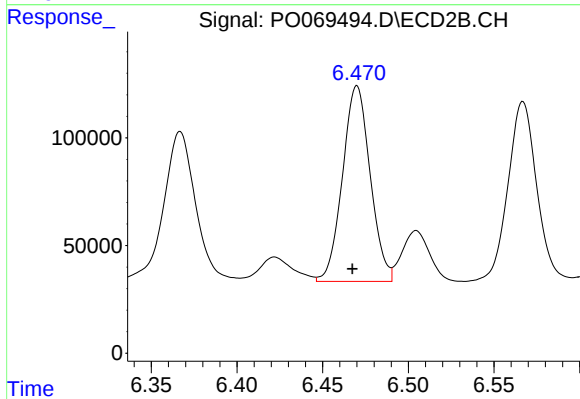

#29 AR-1254-4

R.T.: 6.470 min
Delta R.T.: 0.003 min
Response: 1022073
Conc: 404.44 ng/ml

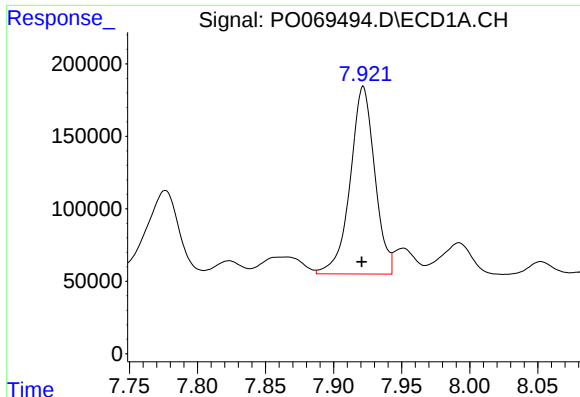


#30 AR-1254-5

R.T.: 7.922 min
Delta R.T.: 0.001 min
Response: 1623178
Conc: 539.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
S5-05-BDL

Manual Integrations
APPROVED

Ankita
7/10/2020 12:33:57 PM

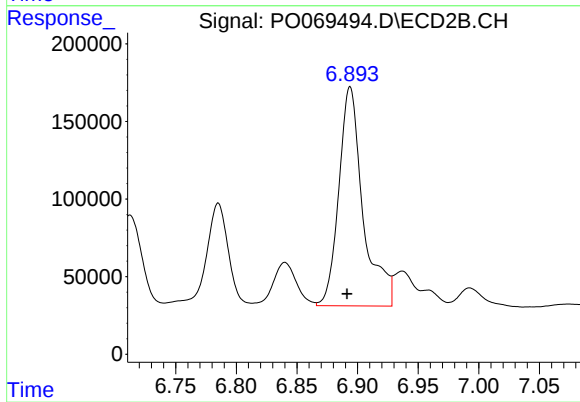

#30 AR-1254-5

R.T.: 6.894 min
Delta R.T.: 0.003 min
Response: 1965304
Conc: 547.60 ng/ml