

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070921\
 Data File : P0079445.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2021 14:09
 Operator : DD\AJ
 Sample : M2987-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-24368

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:41:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	5.022	4.230	641341	270023	9.592	9.416
2)	SA Decachlor...	11.152	9.681	304967	227602	5.996	8.600 #
Target Compounds							
8)	L2 AR-1221-1	5.273	0.000	57687	0	81.412	N.D. #
9)	L2 AR-1221-2	5.379	0.000	7107	0	13.707	N.D. #
12)	L3 AR-1232-2	6.074f	0.000	8846	0	12.277	N.D. #
28)	L6 AR-1254-3	7.899f	0.000	13780	0	3.664	N.D. #
39)	L8 AR-1262-4	0.000	8.557f	0	36294	N.D.	13.525 #
42)	L9 AR-1268-2	0.000	8.557f	0	36294	N.D.	9.746 #
45)	L9 AR-1268-5	0.000	9.390	0	14169	N.D.	1.457 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO070921\
Data File : PO079445.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2021 14:09
Operator : DD\AJ
Sample : M2987-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:41:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

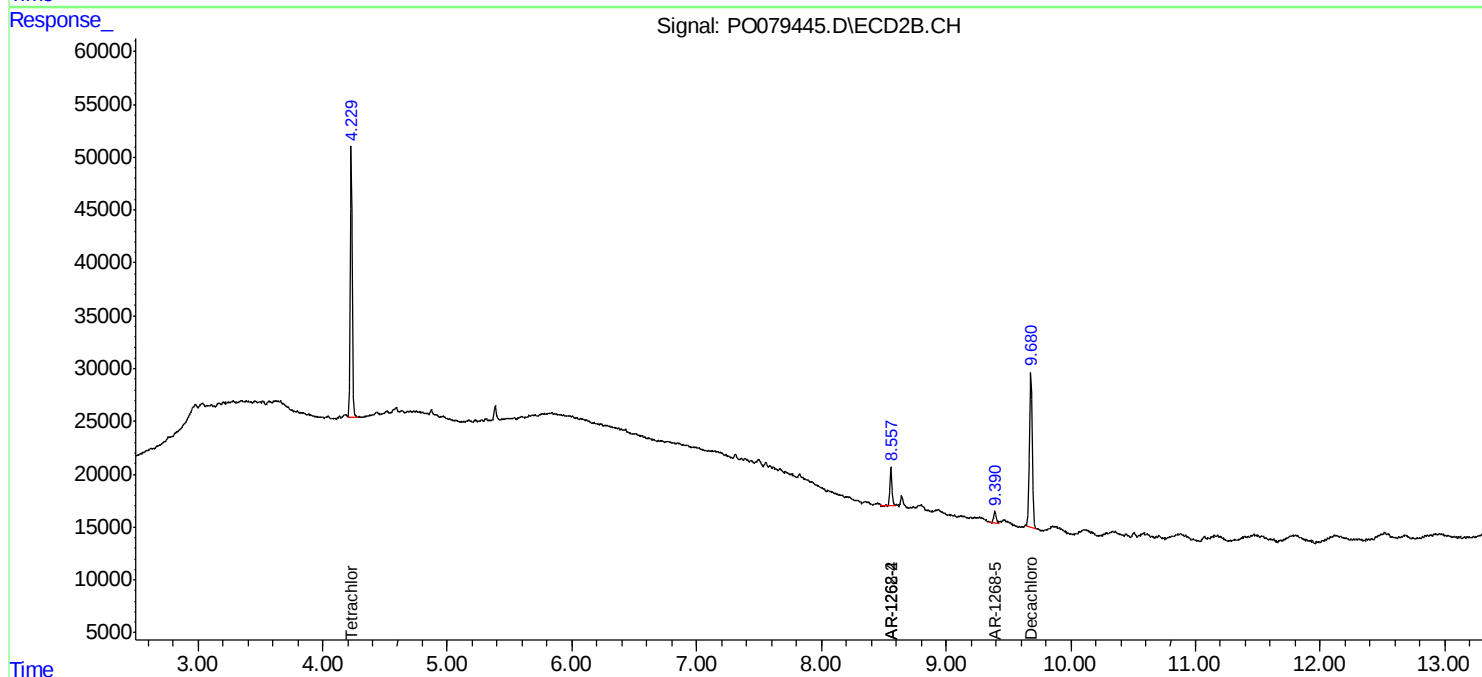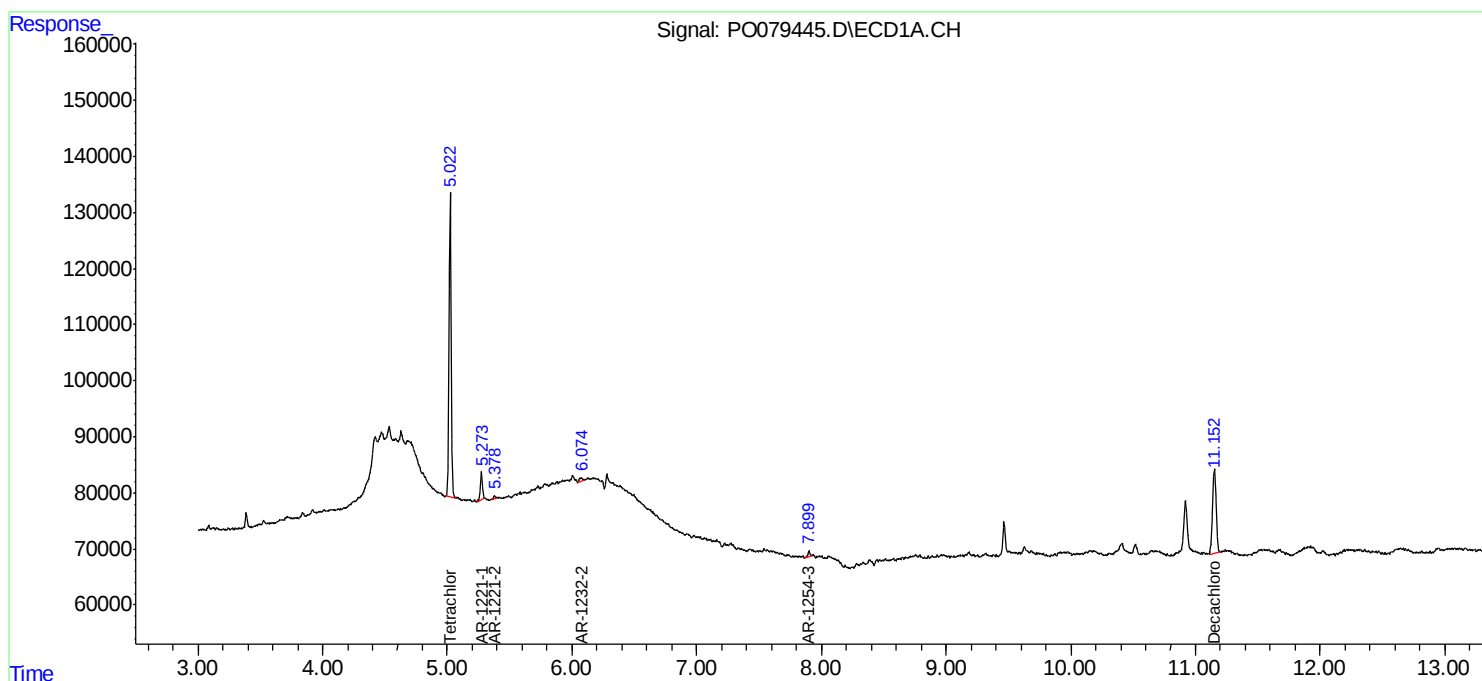


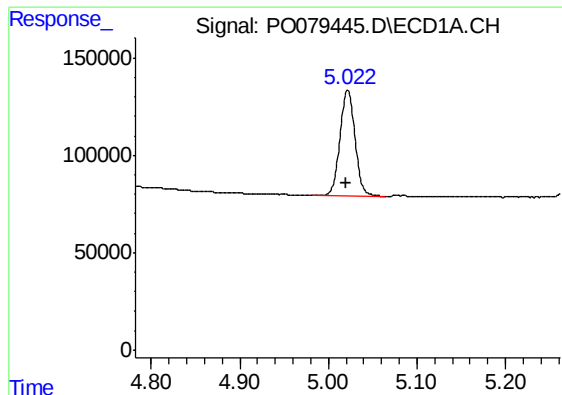

#1 Tetrachloro-m-xylene


R.T.: 5.022 min
Delta R.T.: 0.002 min
Response: 641341
Conc: 9.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

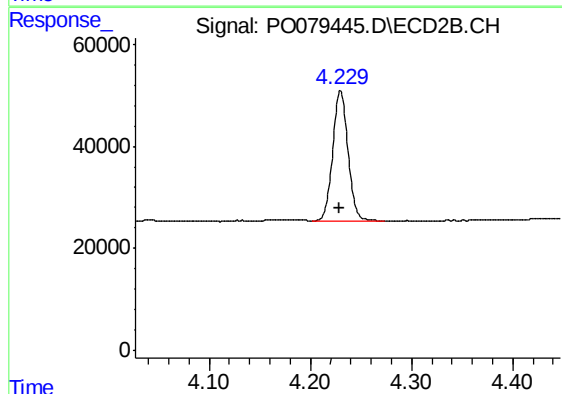


#1 Tetrachloro-m-xylene

R.T.: 4.230 min
Delta R.T.: 0.001 min
Response: 270023
Conc: 9.42 ng/ml

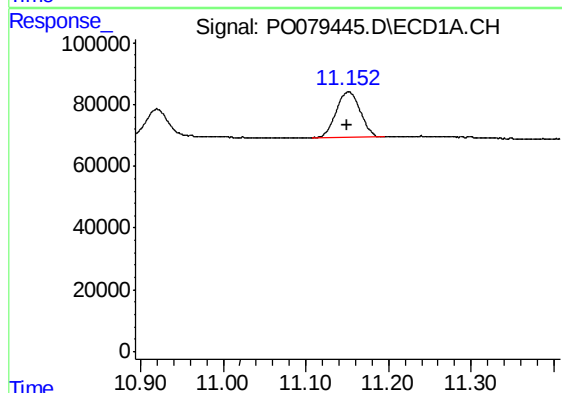


#2 Decachlorobiphenyl

R.T.: 11.152 min
Delta R.T.: 0.002 min
Response: 304967
Conc: 6.00 ng/ml

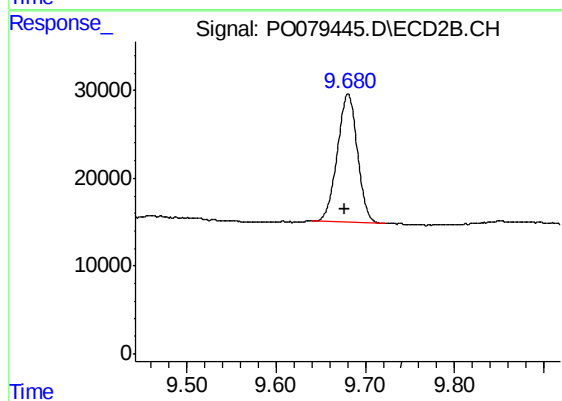

#2 Decachlorobiphenyl


R.T.: 9.681 min
Delta R.T.: 0.003 min
Response: 227602
Conc: 8.60 ng/ml

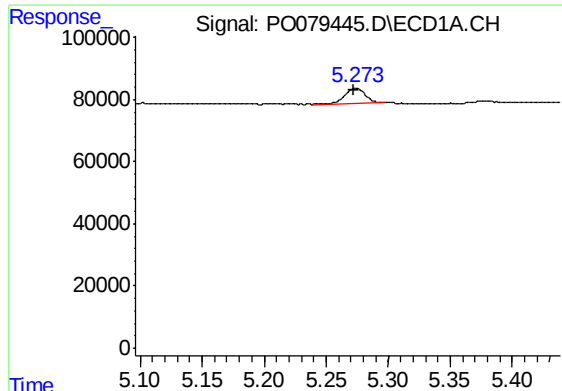

#8 AR-1221-1


R.T.: 5.273 min
Delta R.T.: 0.000 min
Response: 57687
Conc: 81.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

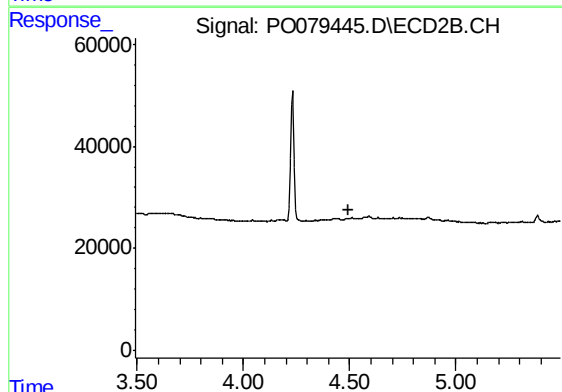


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.492 min
Response: 0
Conc: N.D.

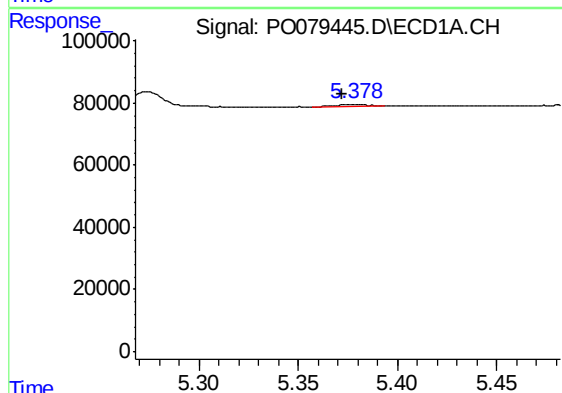


#9 AR-1221-2

R.T.: 5.379 min
Delta R.T.: 0.007 min
Response: 7107
Conc: 13.71 ng/ml

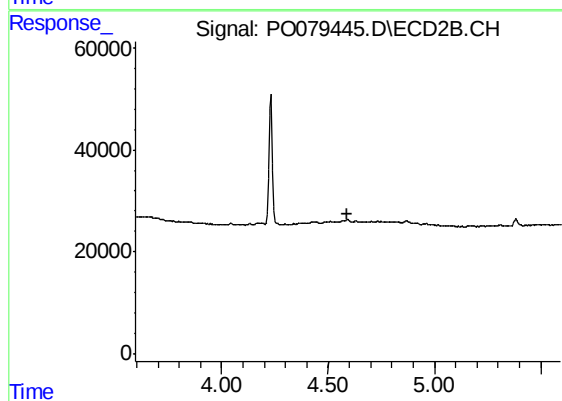

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.593 min
Response: 0
Conc: N.D.

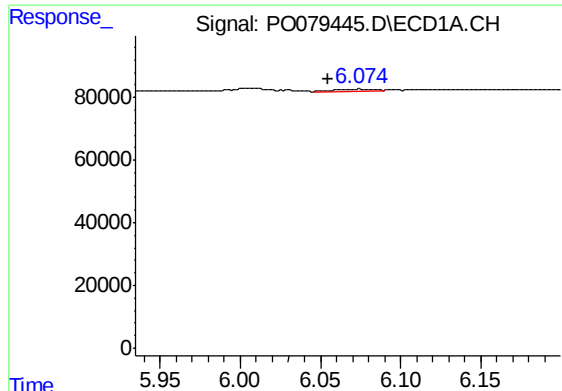

#12 AR-1232-2


R.T.: 6.074 min
Delta R.T.: 0.019 min
Response: 8846
Conc: 12.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

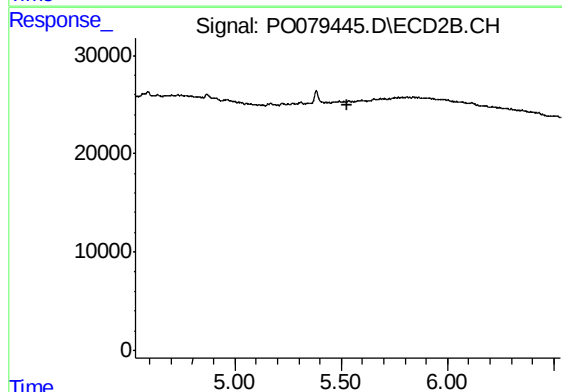


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.532 min
Response: 0
Conc: N.D.

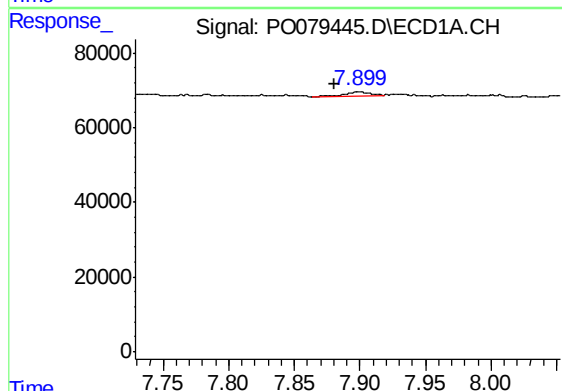


#28 AR-1254-3

R.T.: 7.899 min
Delta R.T.: 0.019 min
Response: 13780
Conc: 3.66 ng/ml

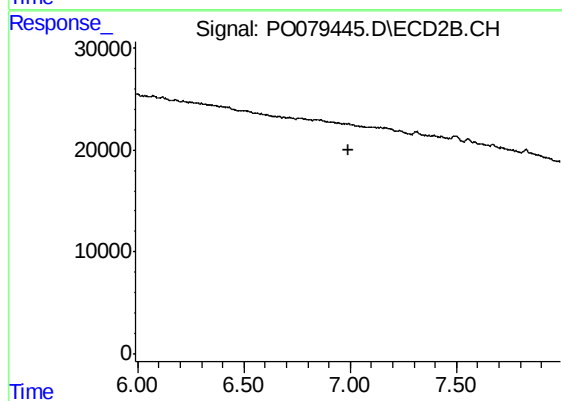

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.990 min
Response: 0
Conc: N.D.

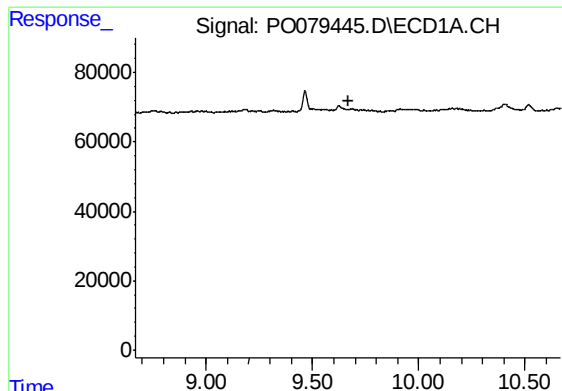

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

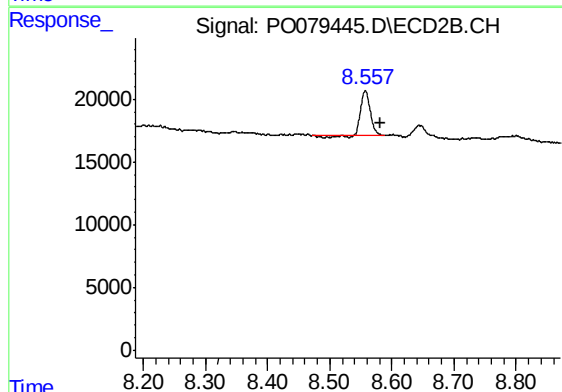


#39 AR-1262-4

R.T.: 8.557 min
Delta R.T.: -0.024 min
Response: 36294
Conc: 13.53 ng/ml

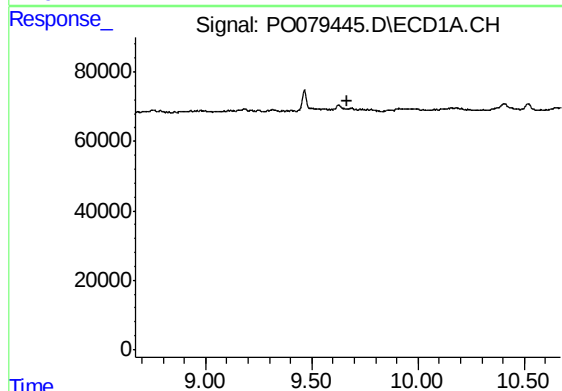


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.670 min
Response: 0
Conc: N.D.

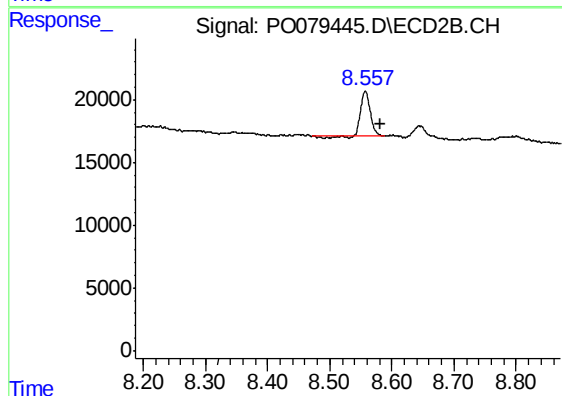

#42 AR-1268-2


R.T.: 8.557 min
Delta R.T.: -0.024 min
Response: 36294
Conc: 9.75 ng/ml

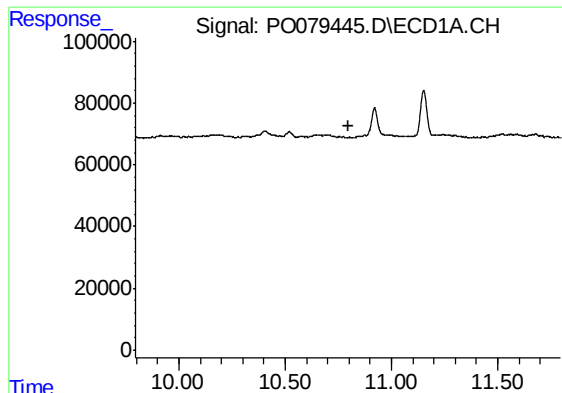

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.795 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CHRT-24368

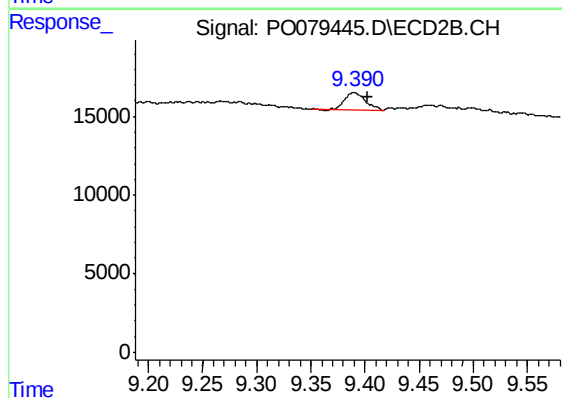

#45 AR-1268-5

R.T.: 9.390 min
Delta R.T.: -0.013 min
Response: 14169
Conc: 1.46 ng/ml