

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070921\
 Data File : P0079441.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Jul 2021 12:59
 Operator : DD\AJ
 Sample : M2928-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TOTE-COMP-64-66

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 01:39:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Jul 10 00:52:22 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.019	4.228	1108232	404784	16.576	14.116
2) SA Decachlor...	11.147	9.679	844690	467851	16.608	17.678

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0070921\
Data File : P0079441.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Jul 2021 12:59
Operator : DD\AJ
Sample : M2928-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-64-66

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 01:39:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070821.M
Quant Title : GC EXTRACTABLES
QLast Update : Sat Jul 10 00:52:22 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

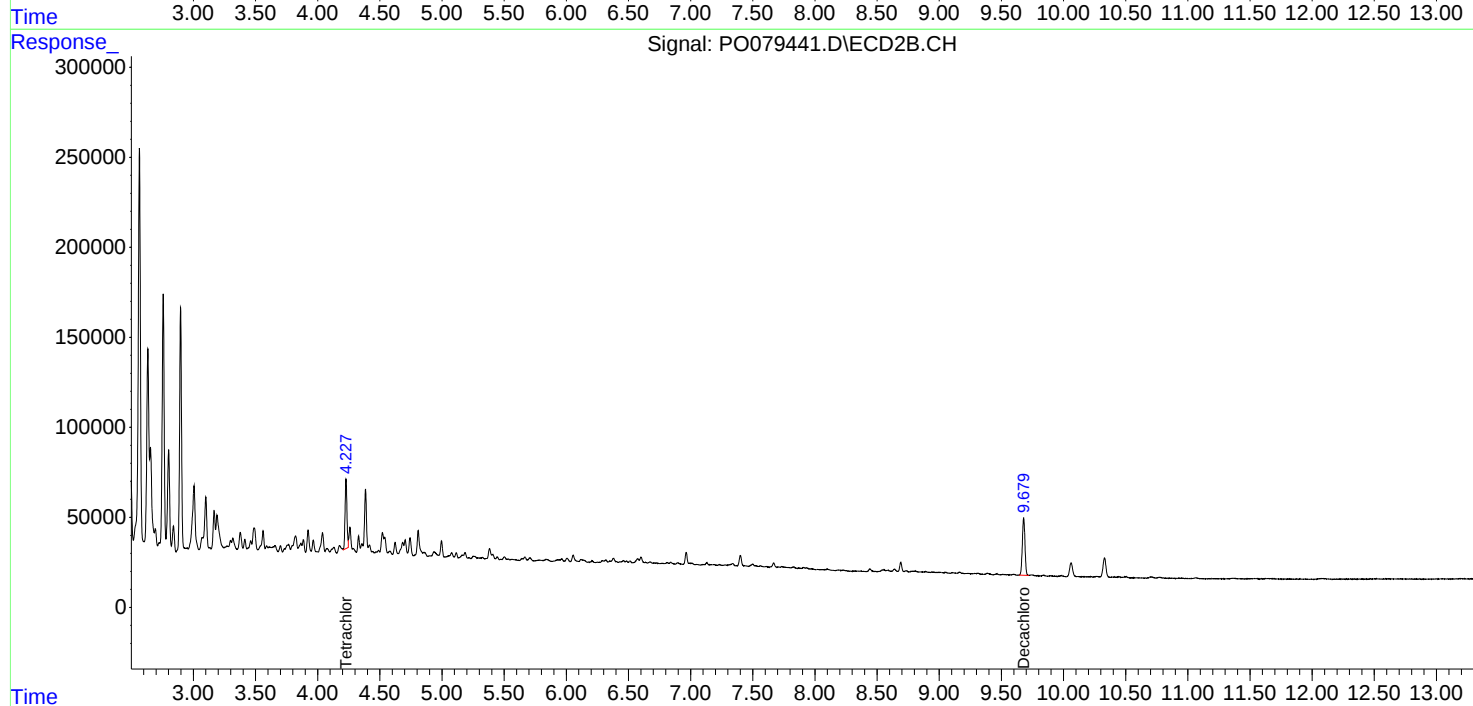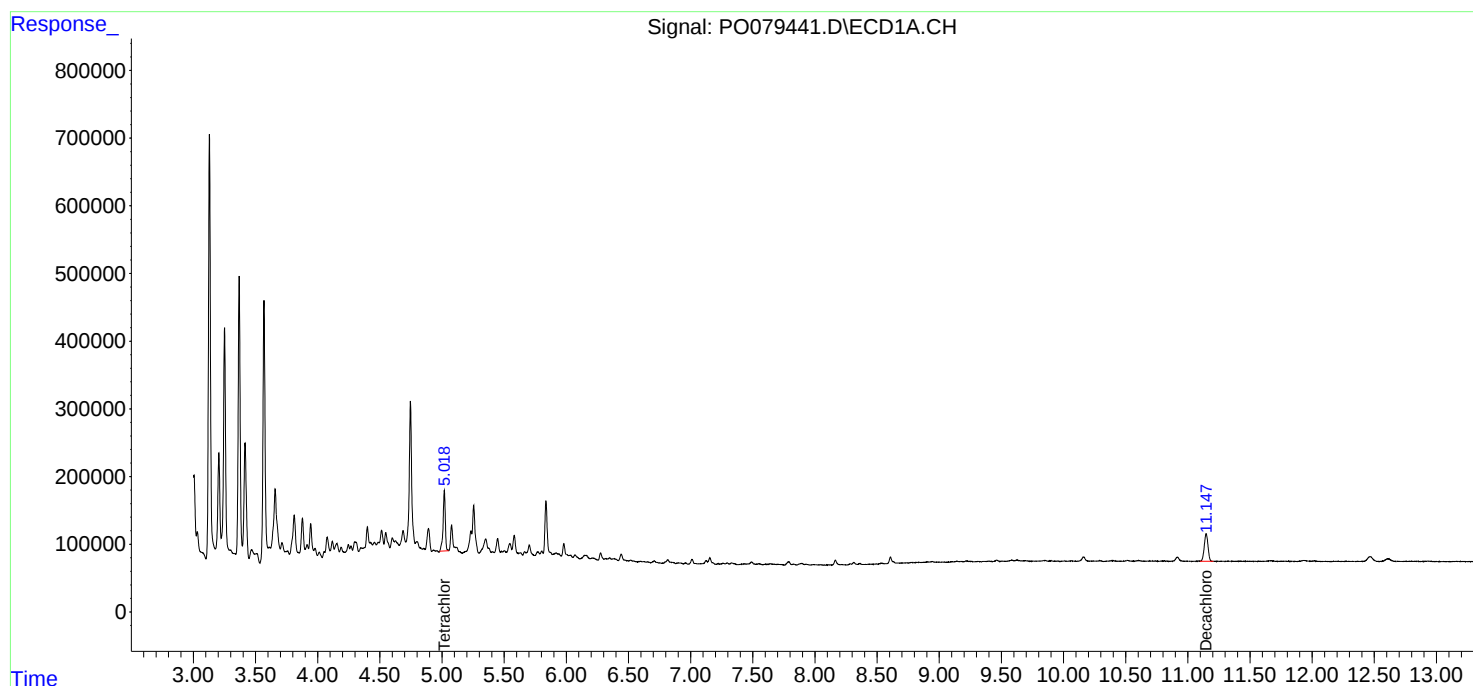


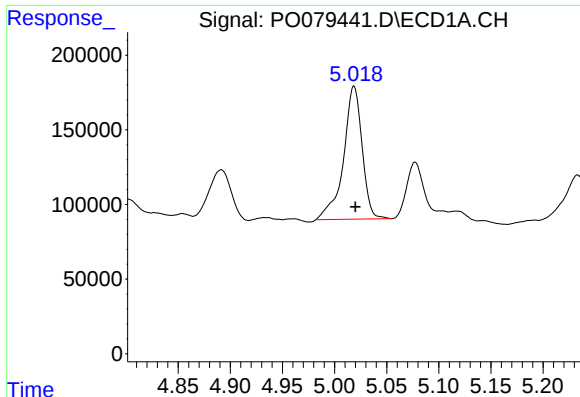

#1 Tetrachloro-m-xylene


R.T.: 5.019 min
Delta R.T.: -0.001 min
Response: 1108232
Conc: 16.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
TOTE-COMP-64-66

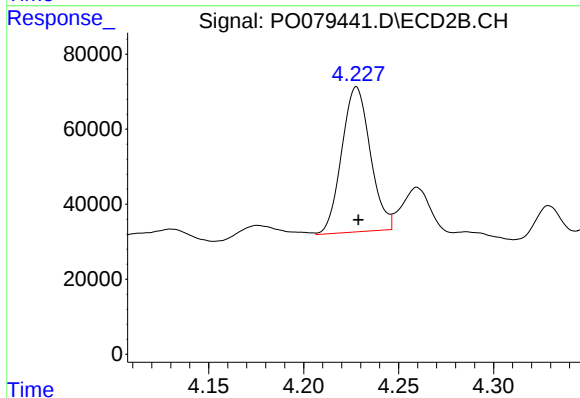


#1 Tetrachloro-m-xylene

R.T.: 4.228 min
Delta R.T.: -0.001 min
Response: 404784
Conc: 14.12 ng/ml

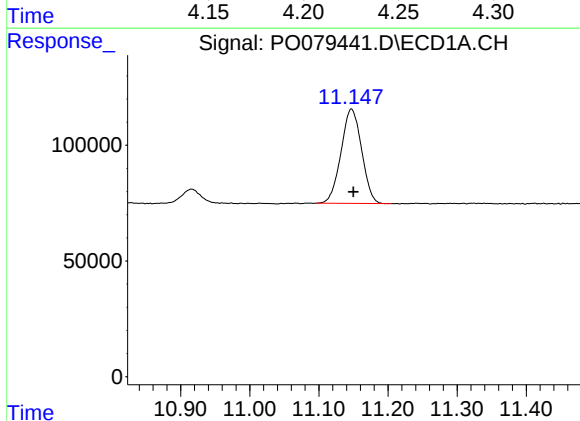

#2 Decachlorobiphenyl

R.T.: 11.147 min
Delta R.T.: -0.003 min
Response: 844690
Conc: 16.61 ng/ml

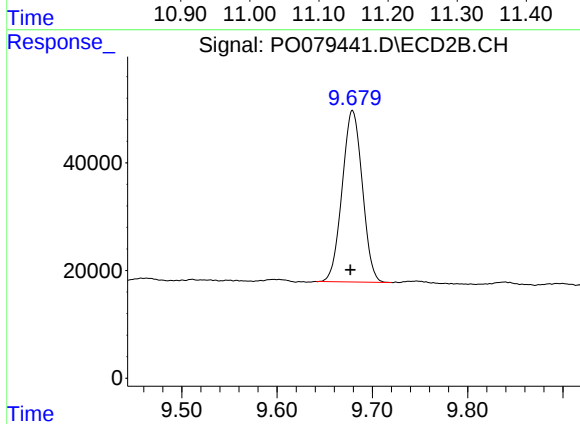

#2 Decachlorobiphenyl

R.T.: 9.679 min
Delta R.T.: 0.002 min
Response: 467851
Conc: 17.68 ng/ml