

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071018\
Data File : P0046545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2018 20:14
Operator : SM/SJ
Sample : J3914-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
B3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 04:03:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.206	3.532	5660381	5231096	23.685	24.628
2)	SA Decachlor...	9.739	8.465	3562801	2877883	18.692	14.836

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071018\
Data File : P0046545.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2018 20:14
Operator : SM/SJ
Sample : J3914-05
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
B3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 04:03:50 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

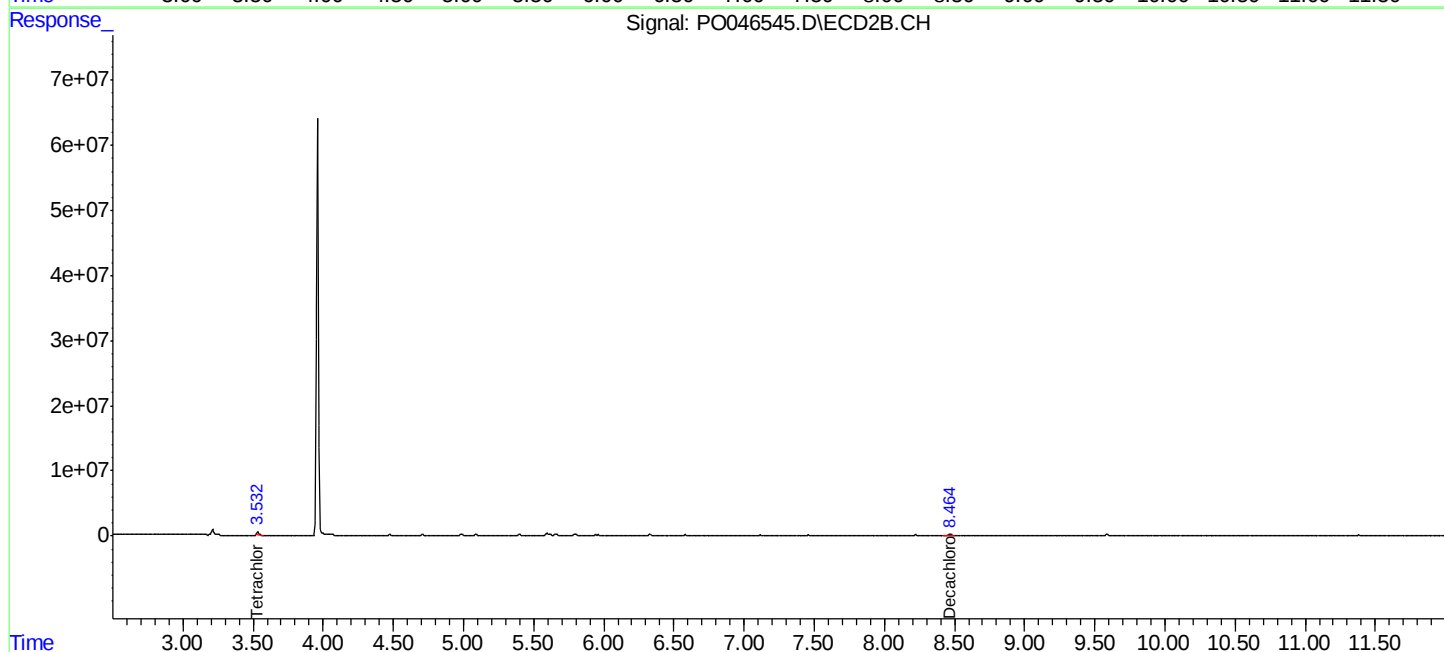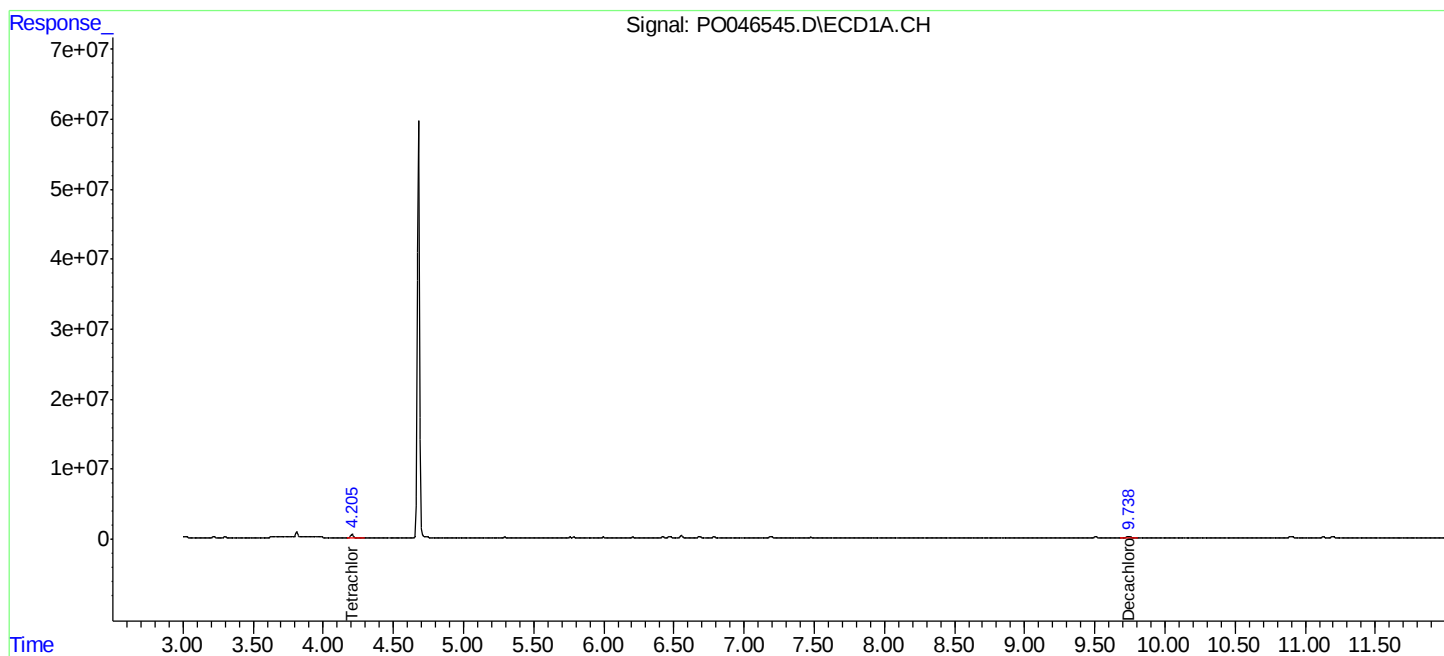


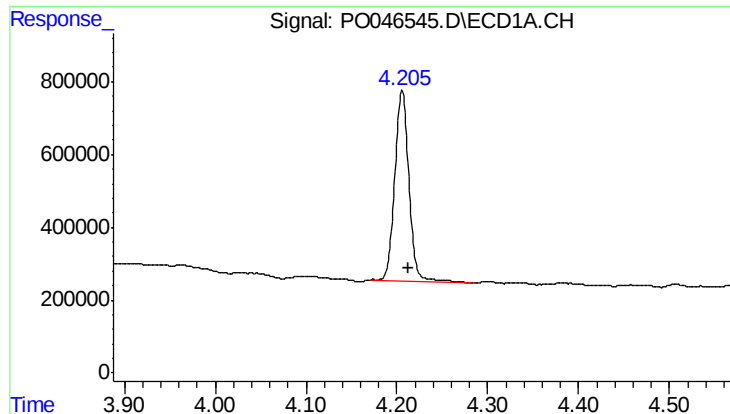

#1 Tetrachloro-m-xylene


R.T.: 4.206 min
Delta R.T.: -0.007 min
Response: 5660381
Conc: 23.69 ng/ml

Instrument :
ECD_O
ClientSampleId :
B3

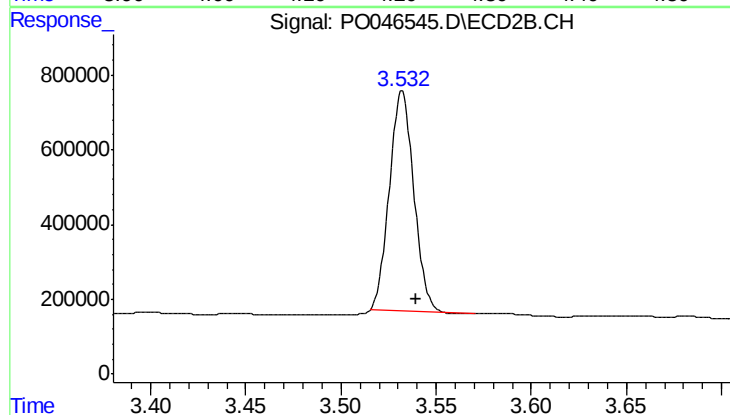


#1 Tetrachloro-m-xylene

R.T.: 3.532 min
Delta R.T.: -0.007 min
Response: 5231096
Conc: 24.63 ng/ml

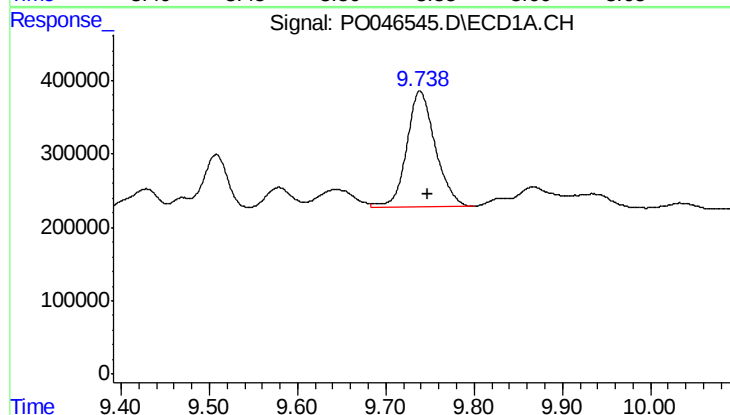

#2 Decachlorobiphenyl

R.T.: 9.739 min
Delta R.T.: -0.009 min
Response: 3562801
Conc: 18.69 ng/ml

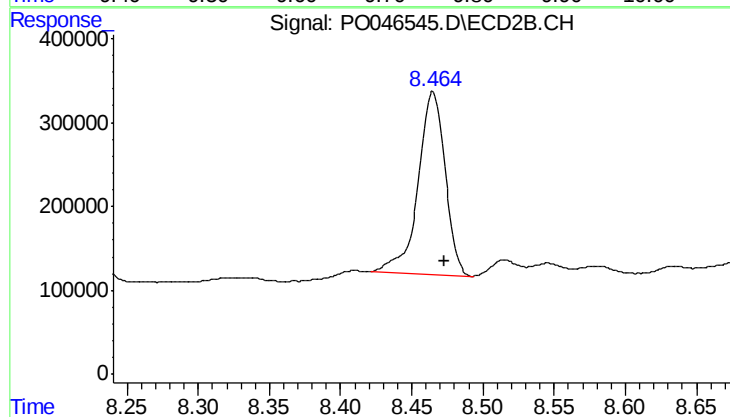

#2 Decachlorobiphenyl

R.T.: 8.465 min
Delta R.T.: -0.008 min
Response: 2877883
Conc: 14.84 ng/ml