

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071018\
Data File : P0046548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2018 21:02
Operator : SM/SJ
Sample : J3914-11
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SMH

Manual Integrations
APPROVED

Sohil
7/11/2018 5:45:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 04:15:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.204	3.531	3421640	4270741	14.317m	20.107m#
2)	SA Decachlor...	9.738	8.465	1276441	1108341	6.697	5.714

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071018\
Data File : P0046548.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2018 21:02
Operator : SM/SJ
Sample : J3914-11
Misc :
ALS Vial : 36 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SMH


Manual Integrations
APPROVED

Sohil
7/11/2018 5:45:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 04:15:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

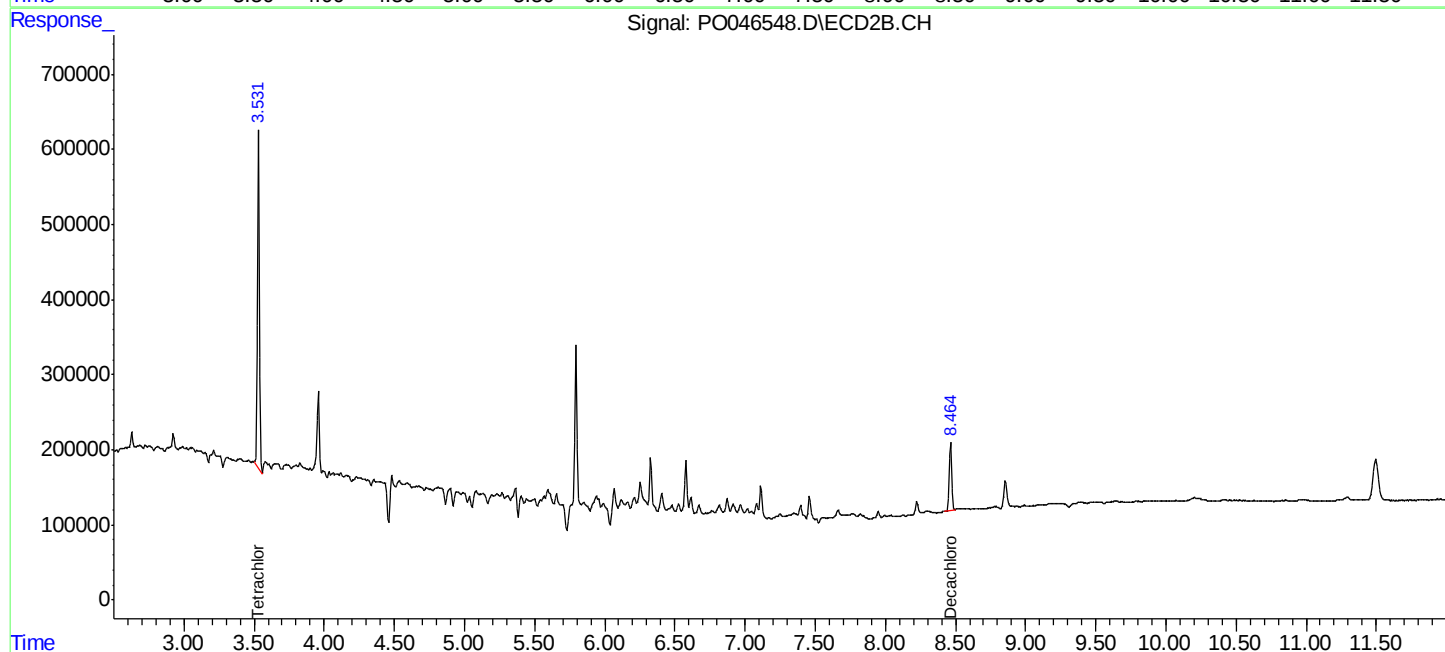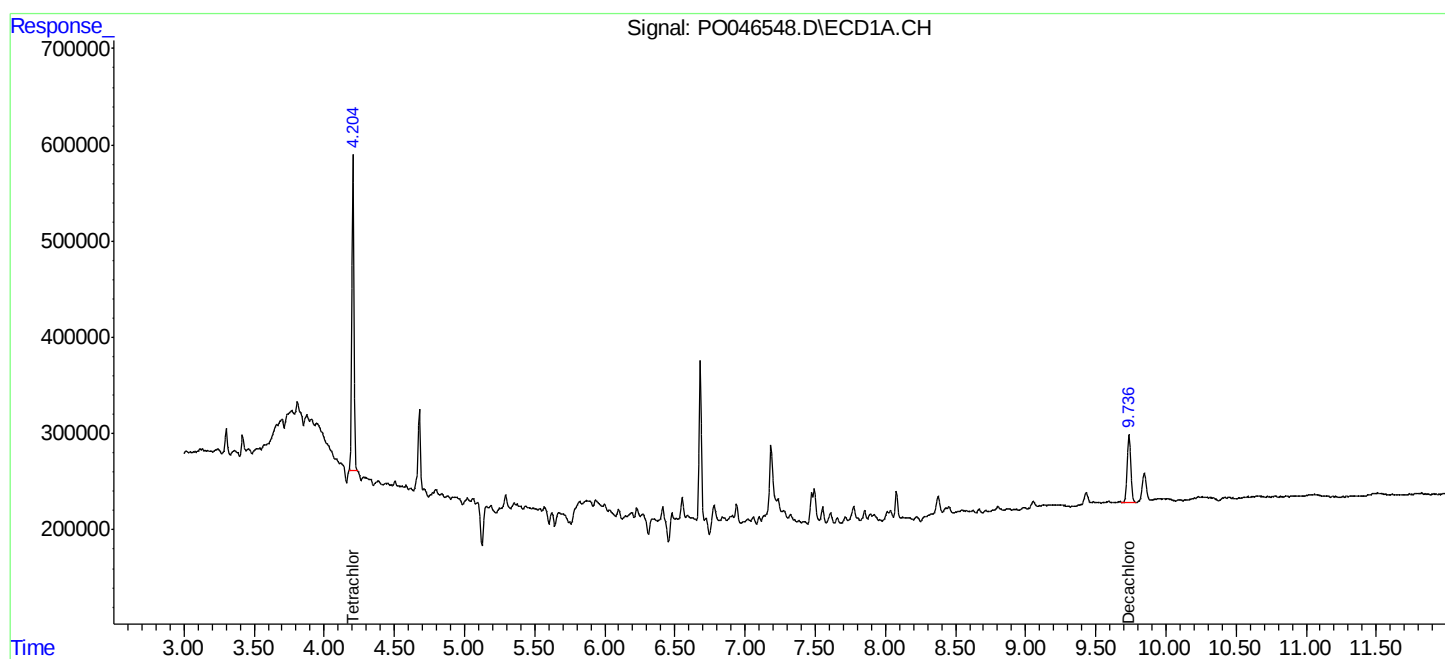

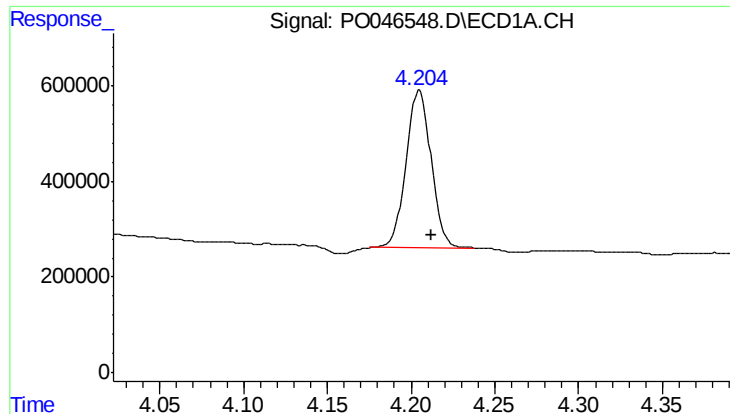


#1 Tetrachloro-m-xylene

R.T.: 4.204 min
Delta R.T.: -0.008 min
Response: 3421640
Conc: 14.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
SMH


Manual Integrations
APPROVED

Sohil
7/11/2018 5:45:25 PM

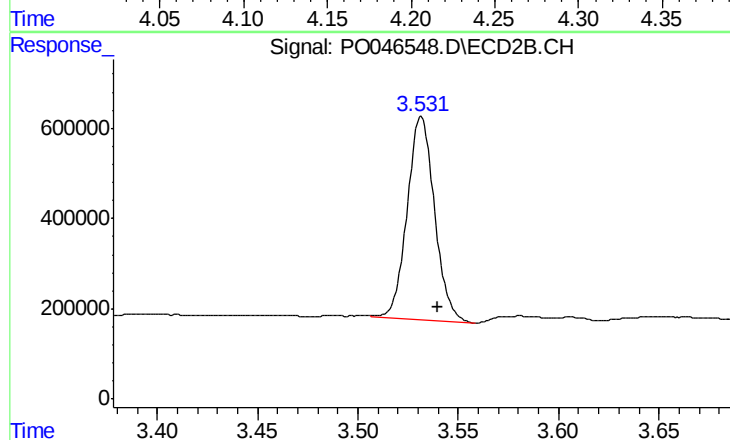


#1 Tetrachloro-m-xylene

R.T.: 3.531 min
Delta R.T.: -0.008 min
Response: 4270741
Conc: 20.11 ng/ml m

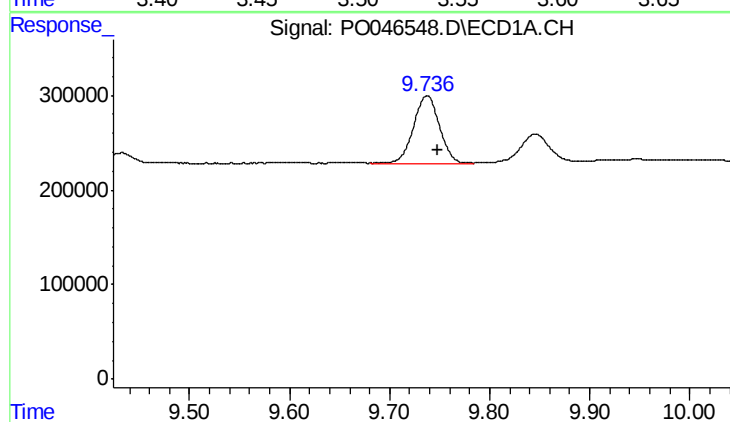

#2 Decachlorobiphenyl

R.T.: 9.738 min
Delta R.T.: -0.010 min
Response: 1276441
Conc: 6.70 ng/ml

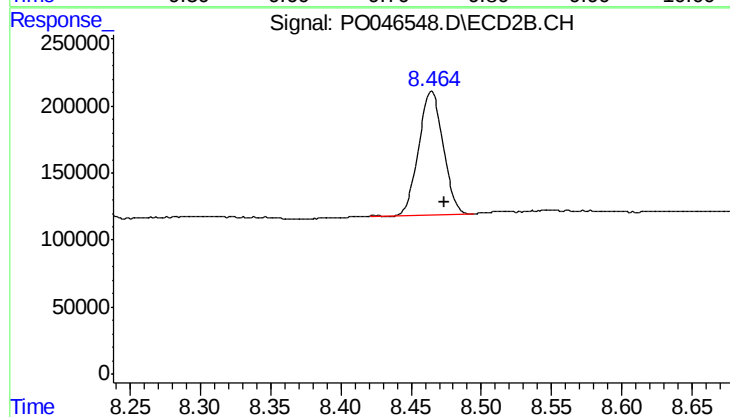

#2 Decachlorobiphenyl

R.T.: 8.465 min
Delta R.T.: -0.009 min
Response: 1108341
Conc: 5.71 ng/ml