

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071018\
Data File : P0046555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 12:32
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 13:06:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.216	3.533	4997974	4723724	20.913	22.239
2) SA Decachlor...	9.748	8.466	3773401	3646799	19.797	18.800

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071018\
Data File : P0046555.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2018 12:32
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 13:06:14 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070718.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Jul 09 15:27:34 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

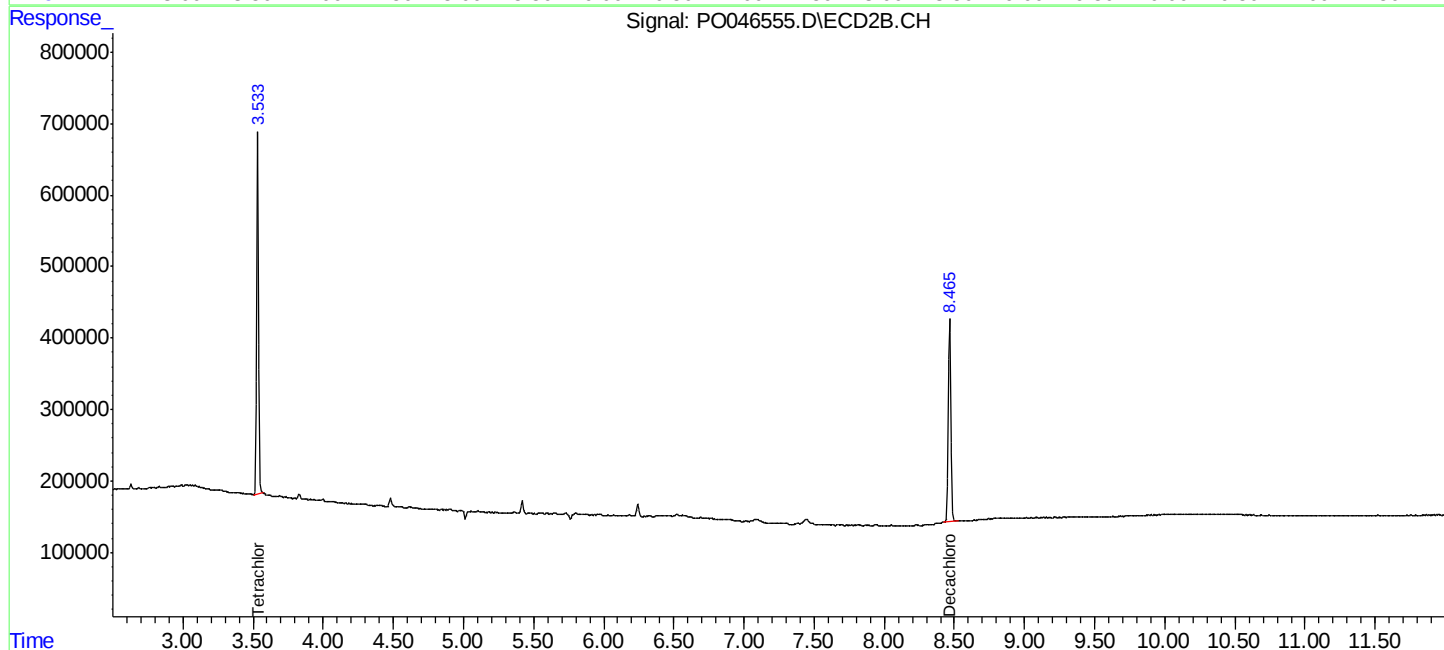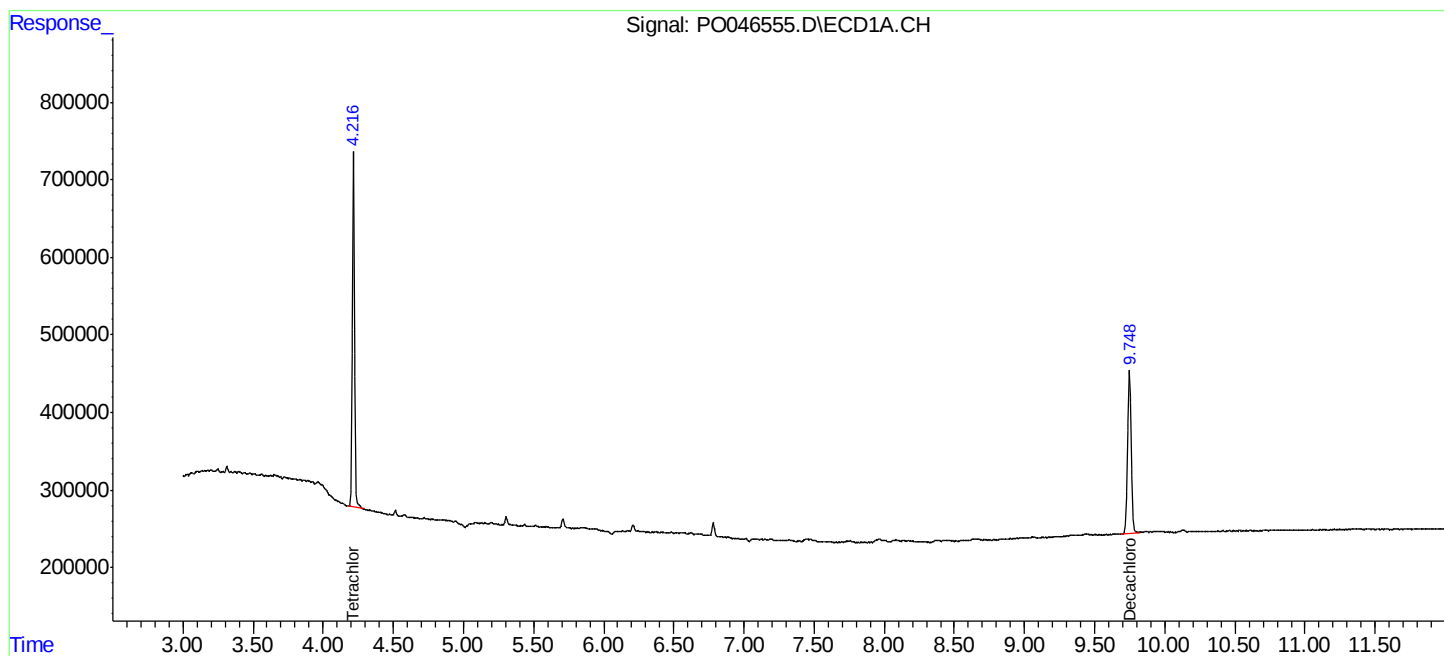


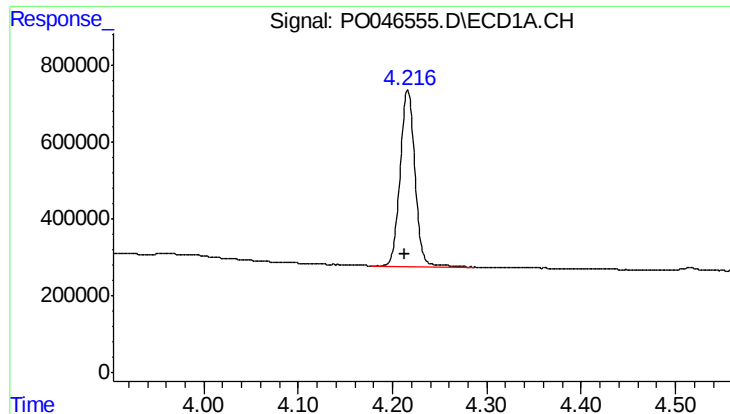

#1 Tetrachloro-m-xylene


R.T.: 4.216 min
Delta R.T.: 0.004 min
Response: 4997974
Conc: 20.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

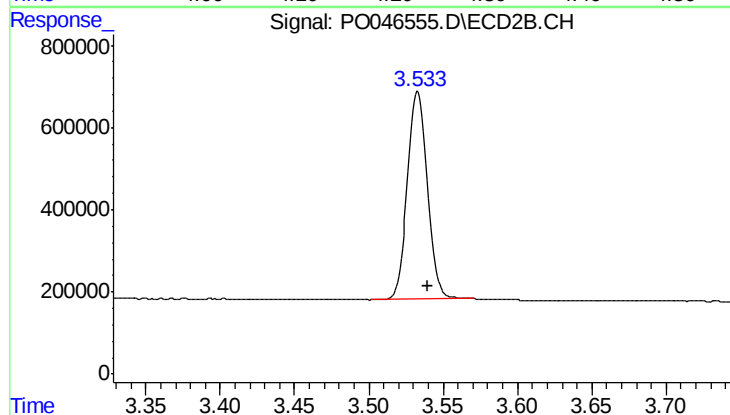


#1 Tetrachloro-m-xylene

R.T.: 3.533 min
Delta R.T.: -0.007 min
Response: 4723724
Conc: 22.24 ng/ml

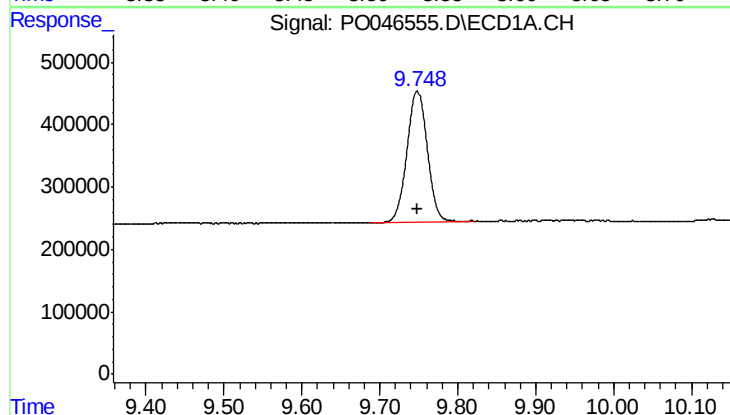

#2 Decachlorobiphenyl

R.T.: 9.748 min
Delta R.T.: 0.000 min
Response: 3773401
Conc: 19.80 ng/ml

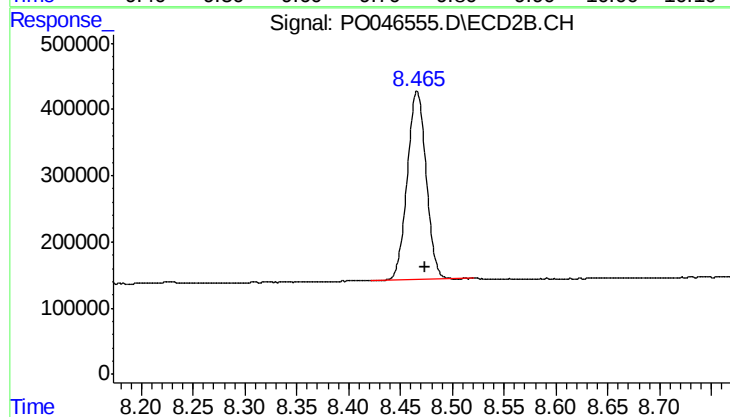

#2 Decachlorobiphenyl

R.T.: 8.466 min
Delta R.T.: -0.007 min
Response: 3646799
Conc: 18.80 ng/ml