

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
 Data File : P0069515.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2020 13:21
 Operator : DD\AJ
 Sample : L3256-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 24465

Manual Integrations
 APPROVED

Ankita
 7/13/2020 3:28:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 16:49:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.394	3.566	895267	977917	23.979	24.573
2) SA Decachlor...	10.060	8.779	1220060	1145224	20.278m	20.179

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
Data File : P0069515.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2020 13:21
Operator : DD\AJ
Sample : L3256-04
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
24465


Manual Integrations
APPROVED

Ankita
7/13/2020 3:28:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 16:49:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

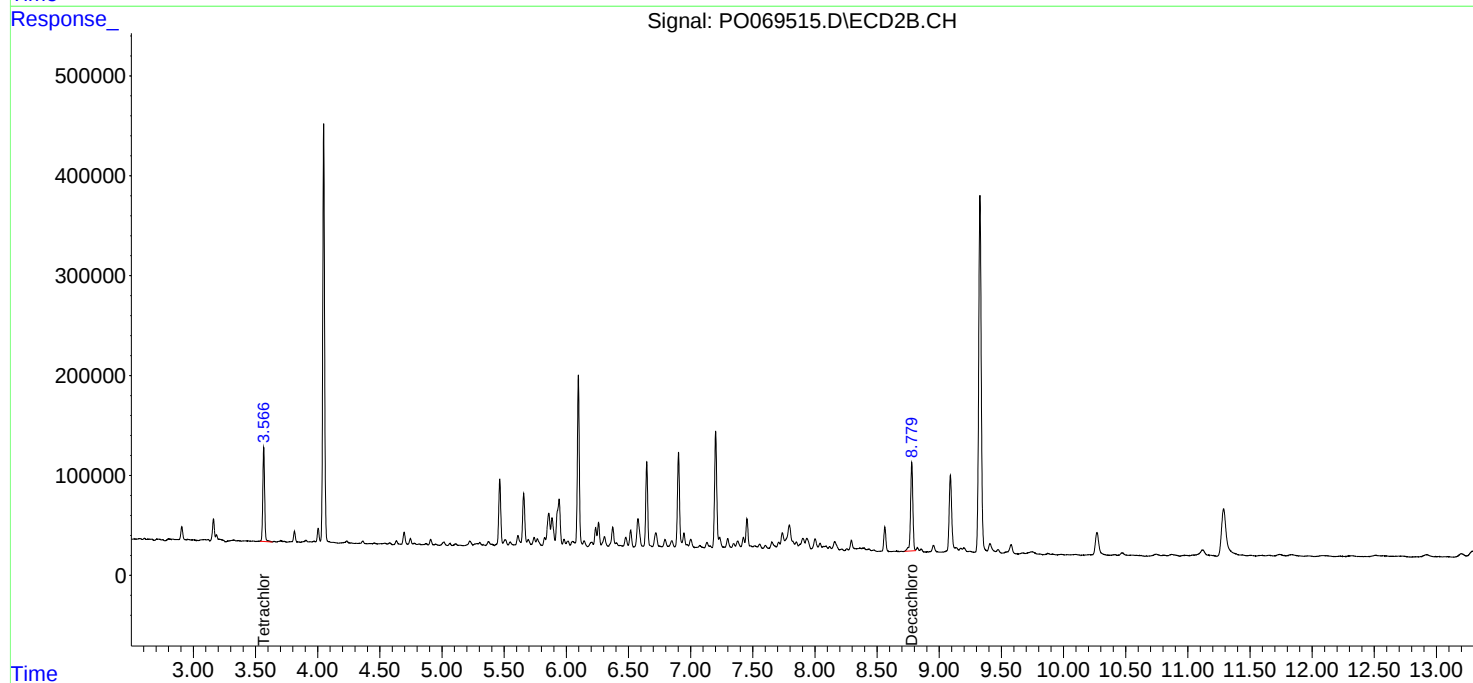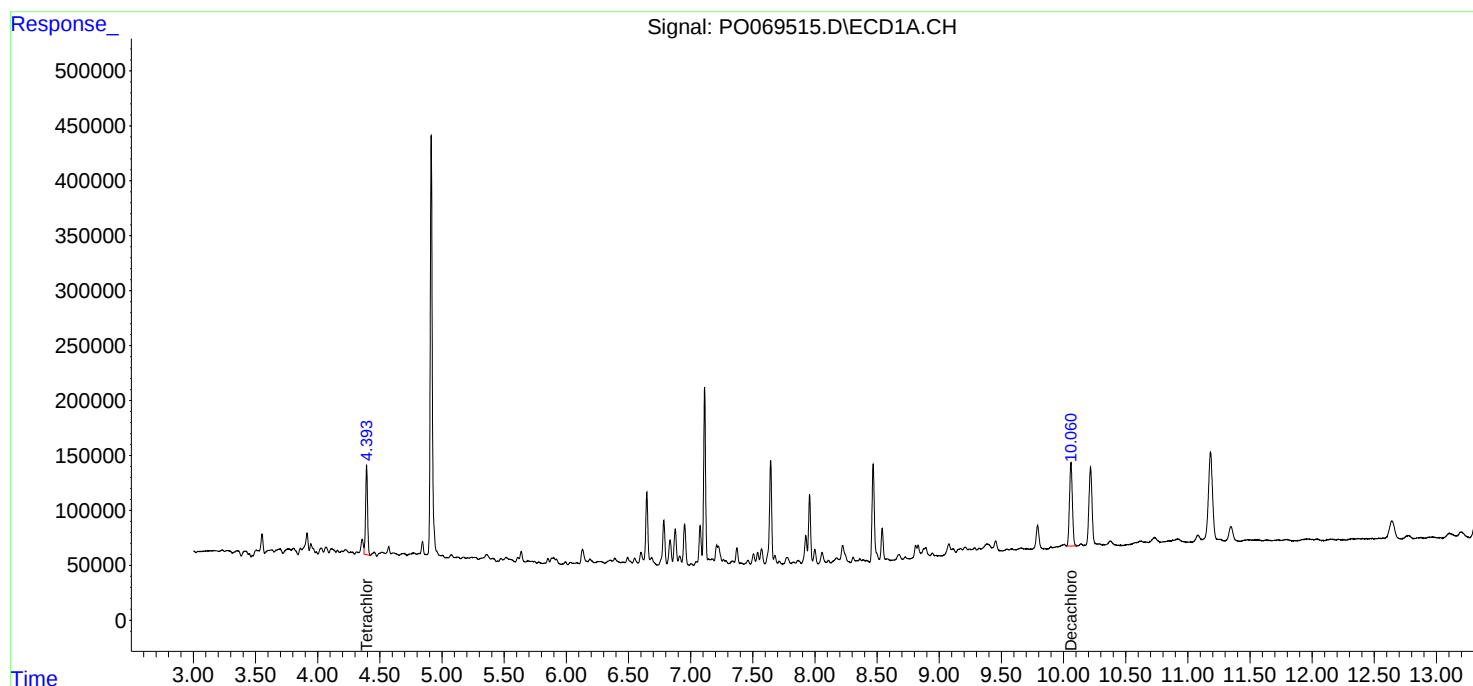

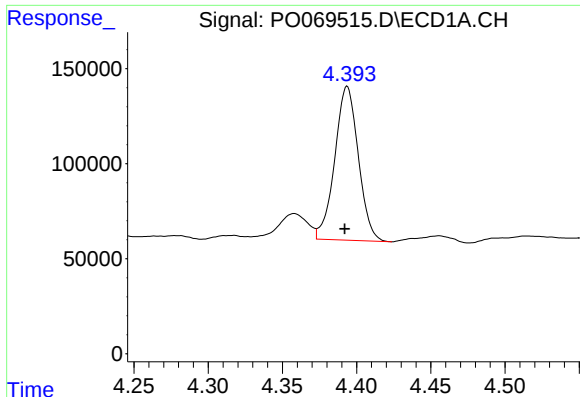


#1 Tetrachloro-m-xylene

R.T.: 4.394 min
Delta R.T.: 0.002 min
Response: 895267
Conc: 23.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
24465


Manual Integrations
APPROVED

Ankita
7/13/2020 3:28:54 PM

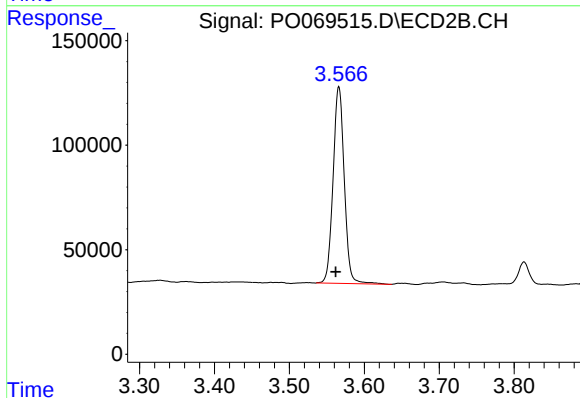


#1 Tetrachloro-m-xylene

R.T.: 3.566 min
Delta R.T.: 0.004 min
Response: 977917
Conc: 24.57 ng/ml

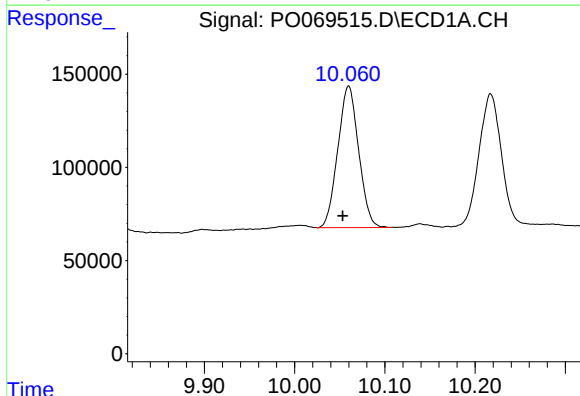

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: 0.006 min
Response: 1220060
Conc: 20.28 ng/ml m

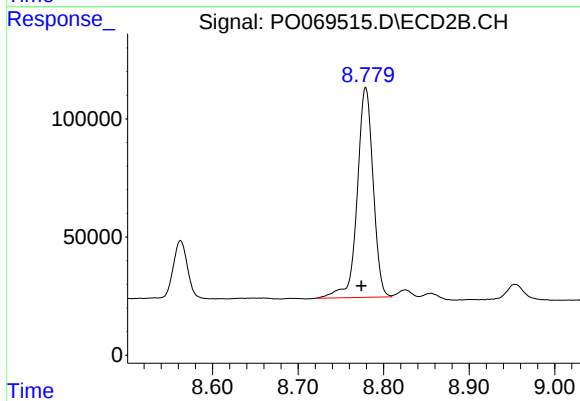

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: 0.005 min
Response: 1145224
Conc: 20.18 ng/ml