

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
 Data File : P0069527.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Jul 2020 17:54
 Operator : DD\AJ
 Sample : L3255-06
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-58

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 11 00:52:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 08 16:12:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.398	3.572	611637	707598	16.382	17.780
2) SA Decachlor...	10.060	8.777	1178320	1003024	19.584	17.673

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
Data File : P0069527.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Jul 2020 17:54
Operator : DD\AJ
Sample : L3255-06
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CHRT-58

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 00:52:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

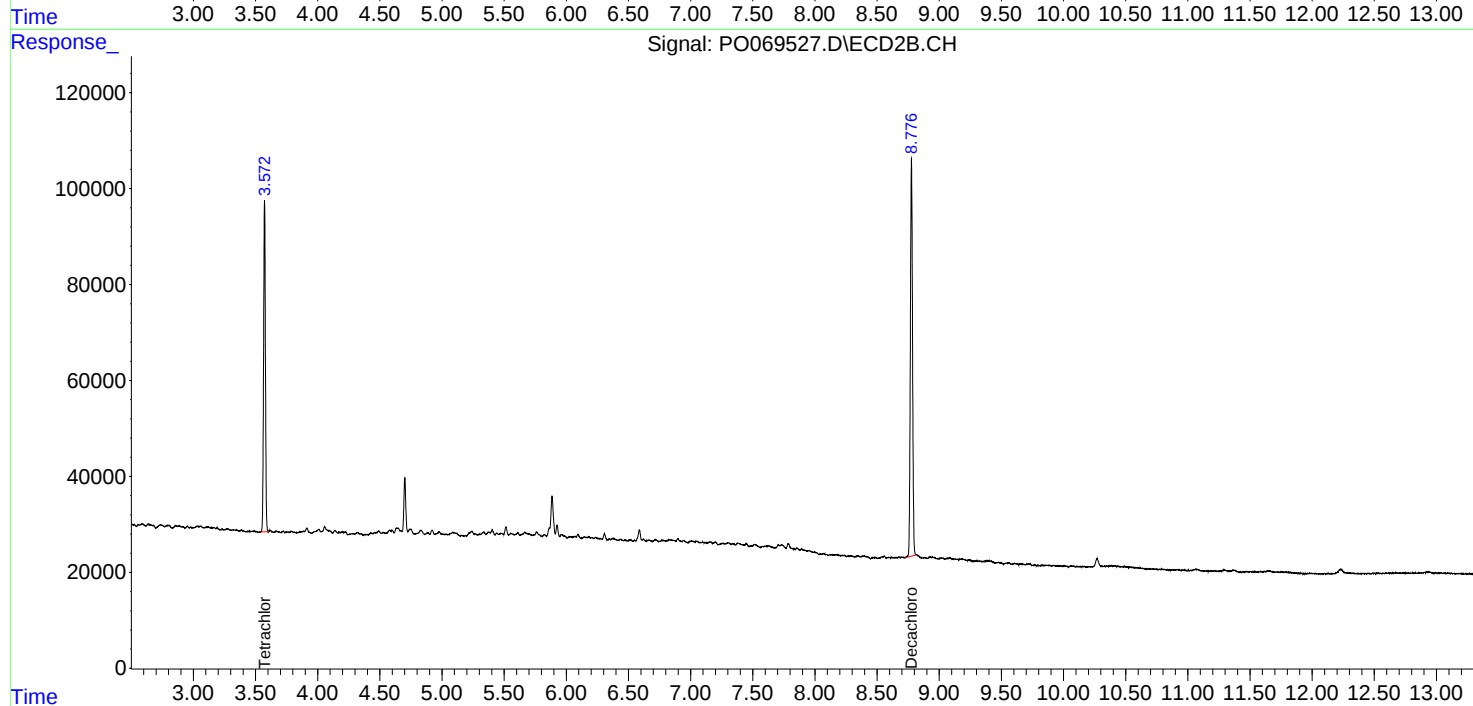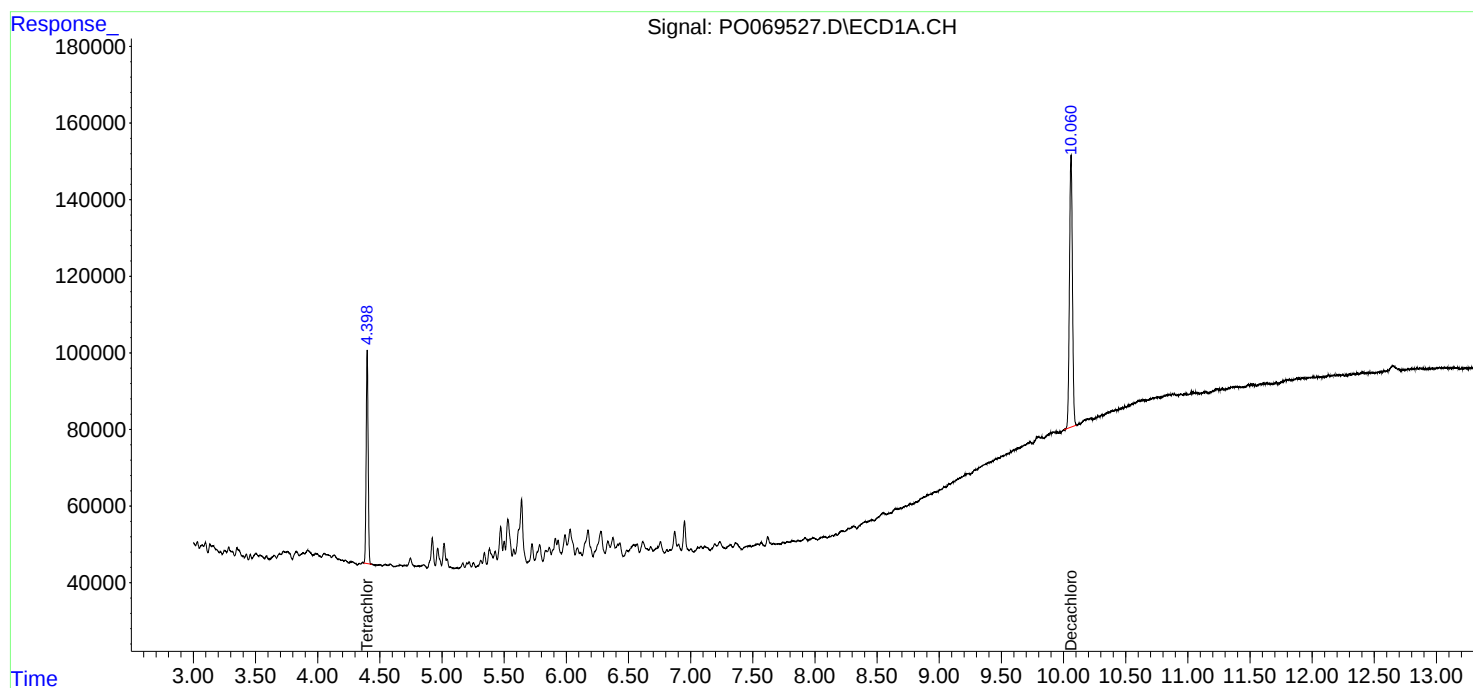


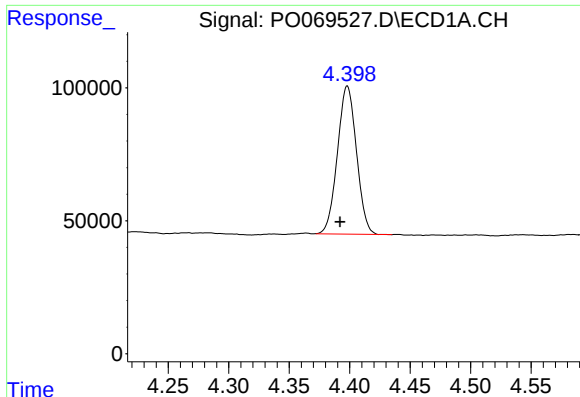

#1 Tetrachloro-m-xylene


R.T.: 4.398 min
Delta R.T.: 0.006 min
Response: 611637
Conc: 16.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-58

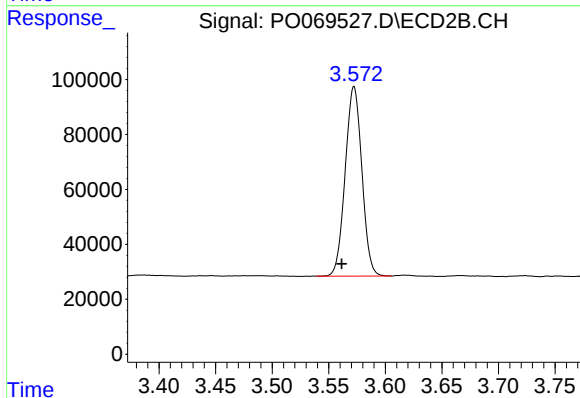


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: 0.011 min
Response: 707598
Conc: 17.78 ng/ml

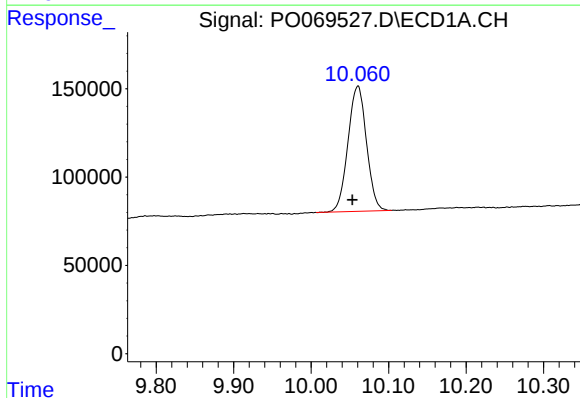

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: 0.007 min
Response: 1178320
Conc: 19.58 ng/ml

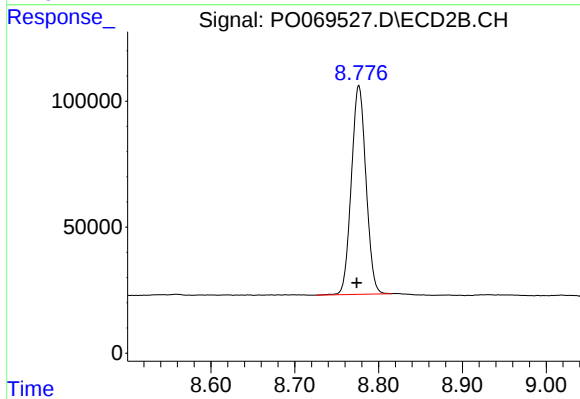

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: 0.002 min
Response: 1003024
Conc: 17.67 ng/ml