

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
Data File : P0069549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2020 00:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 01:57:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.393	3.564	878571	896512	23.532	22.528
2) SA Decachlor...	10.055	8.775	1273569	1115364	21.167	19.653

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0071020\
Data File : P0069549.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Jul 2020 00:47
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 11 01:57:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0070820.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 08 16:12:41 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

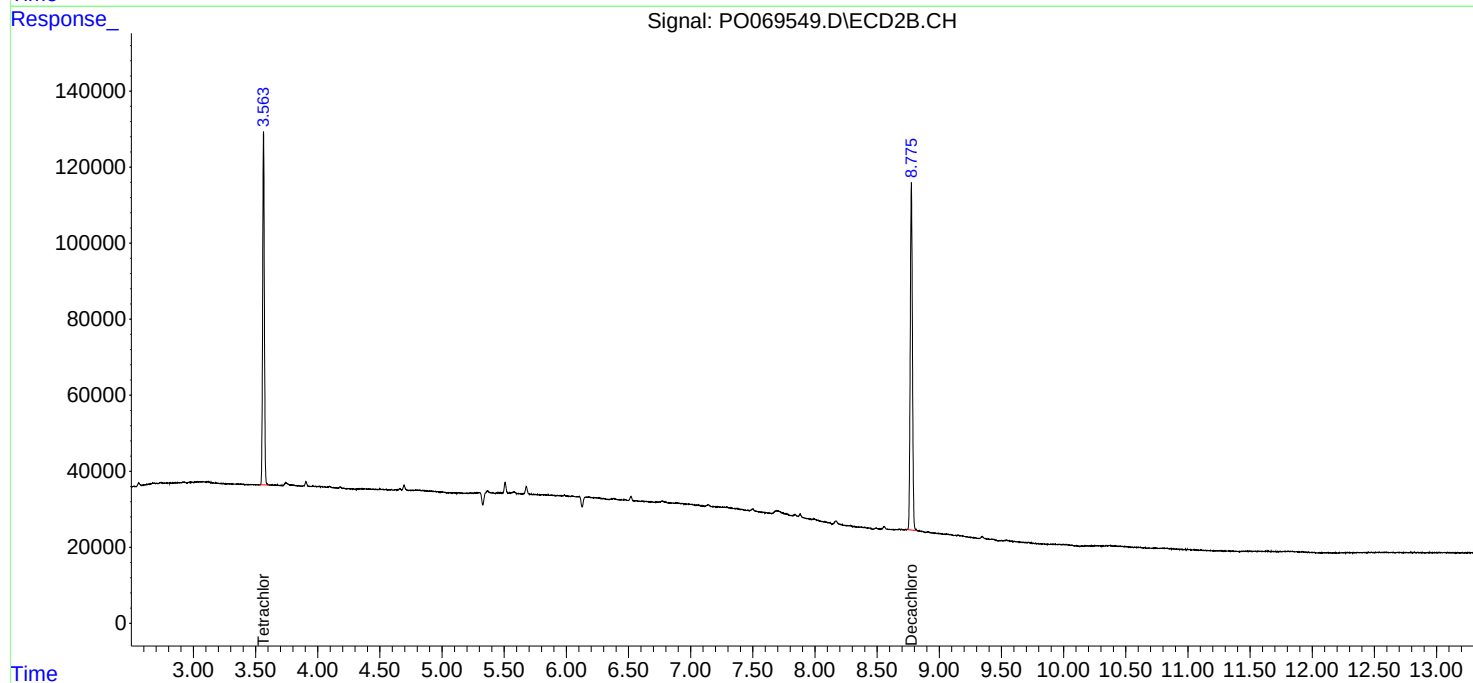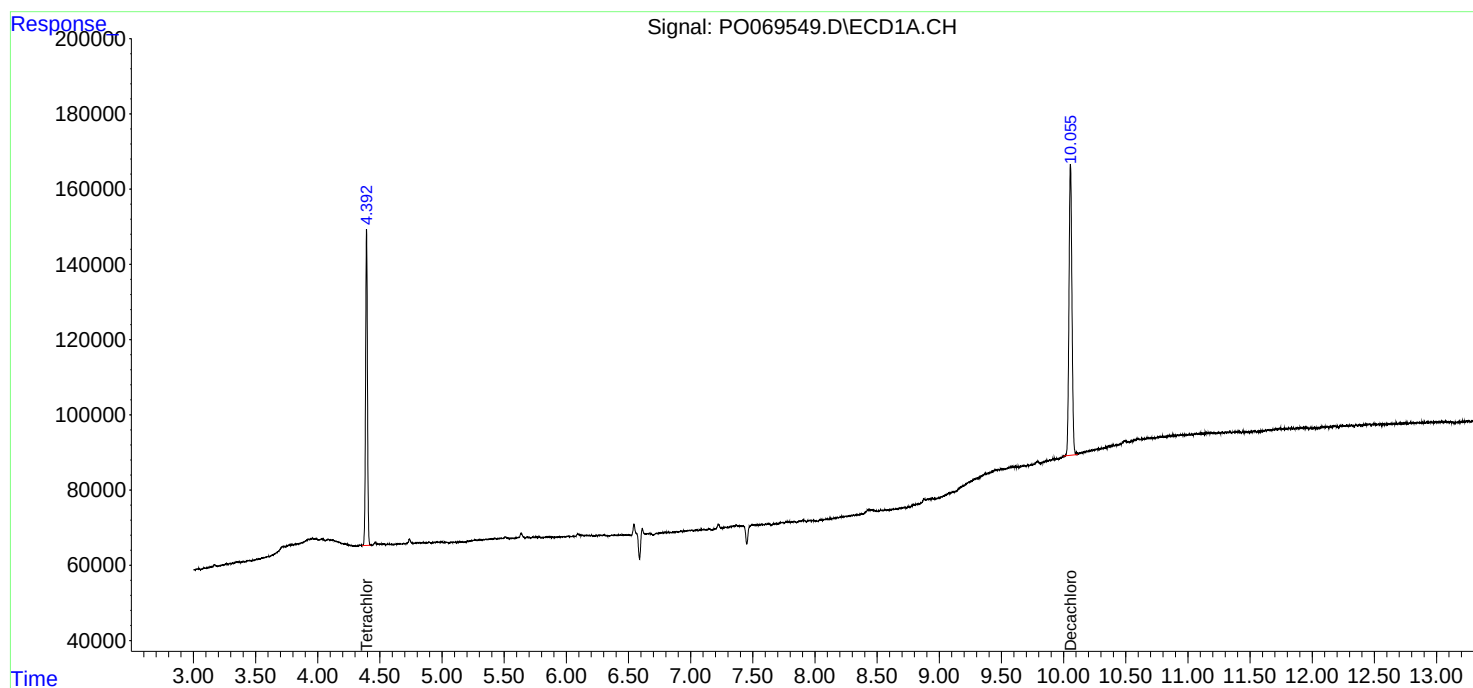


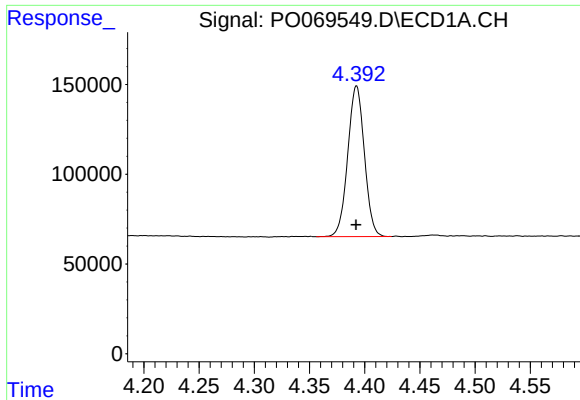

#1 Tetrachloro-m-xylene


R.T.: 4.393 min
Delta R.T.: 0.000 min
Response: 878571
Conc: 23.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

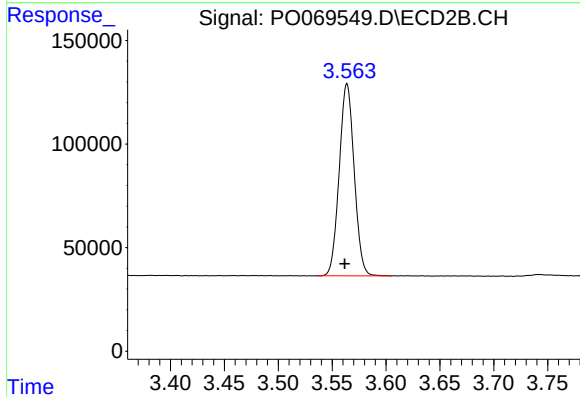


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: 0.002 min
Response: 896512
Conc: 22.53 ng/ml

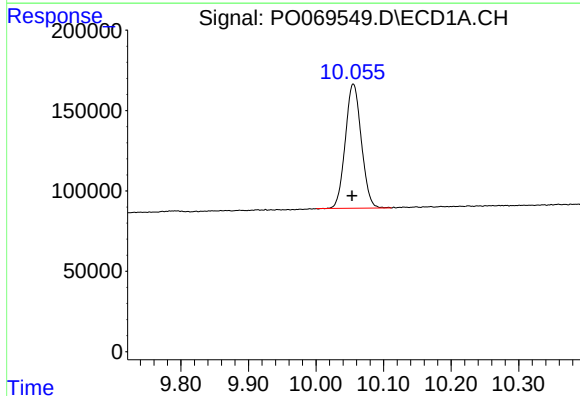

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: 0.002 min
Response: 1273569
Conc: 21.17 ng/ml

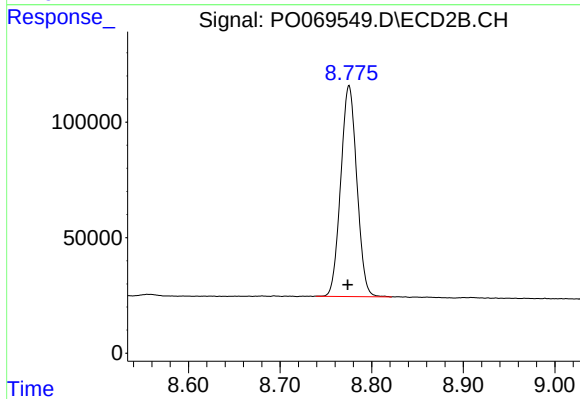

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: 0.001 min
Response: 1115364
Conc: 19.65 ng/ml