

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0071025\
 Data File : P0112195.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Jul 2025 16:07
 Operator : YP/AJ
 Sample : Q2550-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 VNJ-203

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/11/2025
 Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 10 22:53:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0070825.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 09 10:50:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.671	3.666	225.2E6	129.9E6	22.757	20.387
2) SA Decachlor...	8.698	8.647	75133367	24784538	10.989m	14.381m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO071025\
Data File : PO112195.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Jul 2025 16:07
Operator : YP/AJ
Sample : Q2550-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
VNJ-203


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2025
Supervised By :mohammad ahmed 07/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 10 22:53:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO070825.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Jul 09 10:50:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

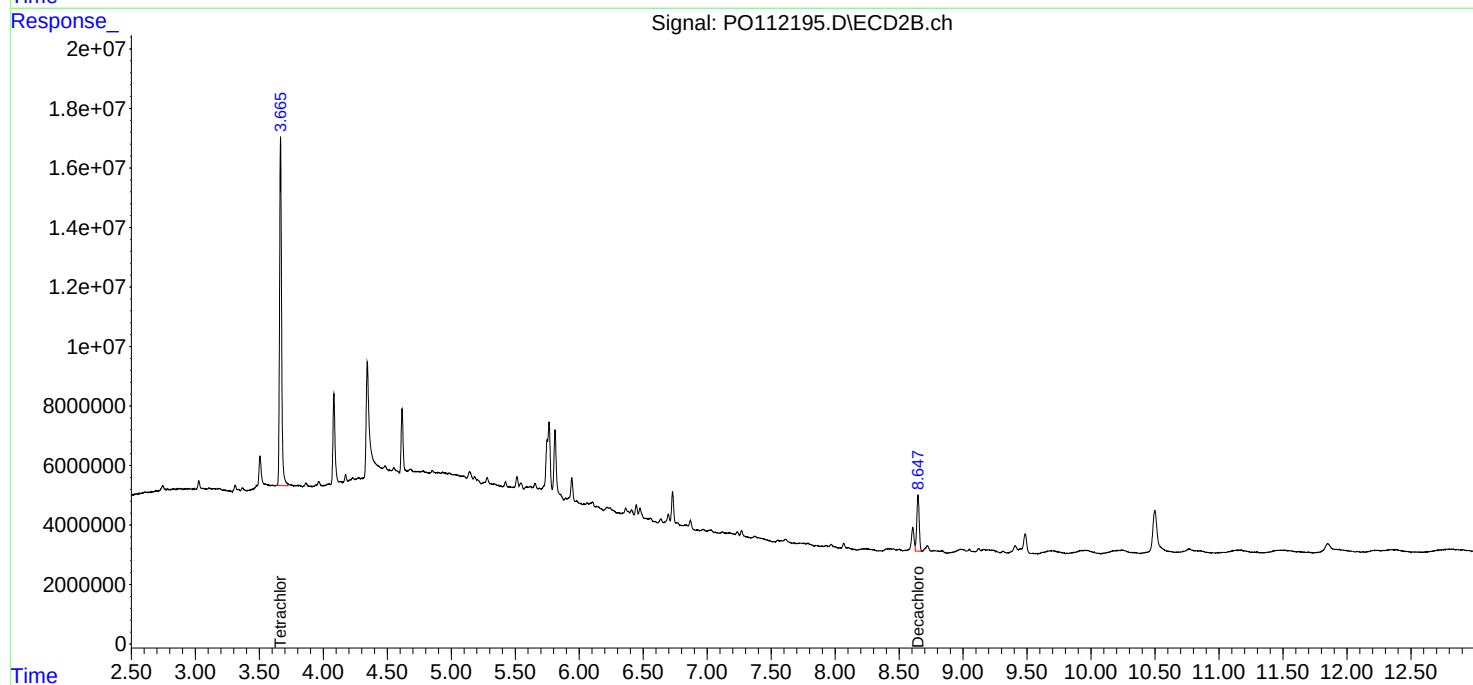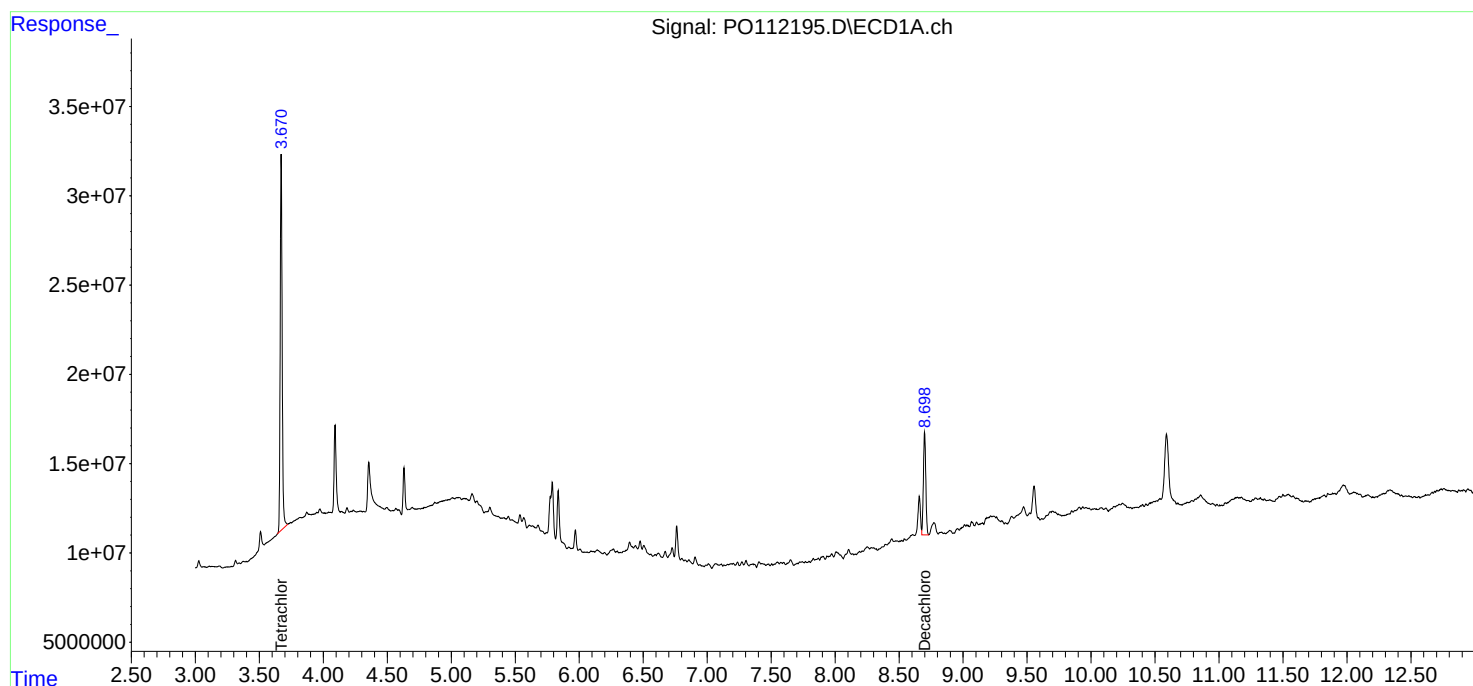

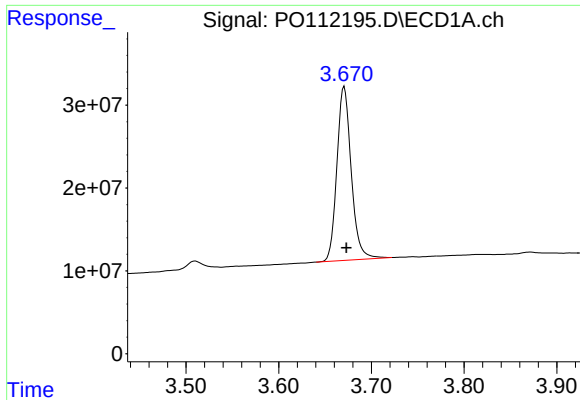


#1 Tetrachloro-m-xylene

R.T.: 3.671 min
Delta R.T.: -0.002 min
Response: 225178078
Conc: 22.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
VNJ-203


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/11/2025
Supervised By :mohammad ahmed 07/11/2025

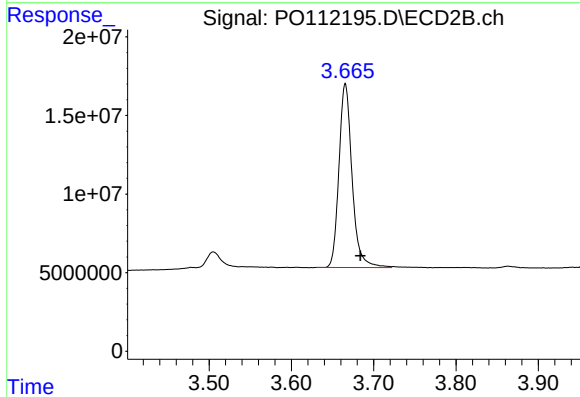


#1 Tetrachloro-m-xylene

R.T.: 3.666 min
Delta R.T.: -0.018 min
Response: 129885522
Conc: 20.39 ng/ml

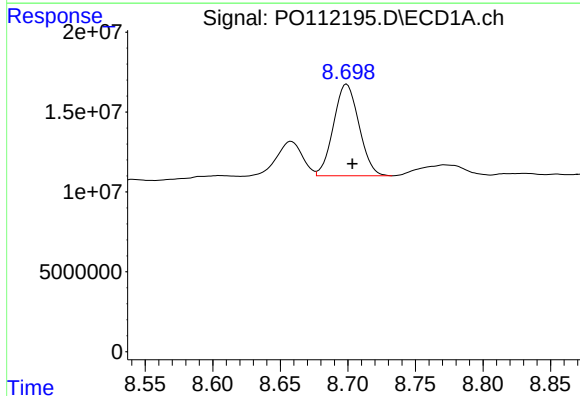

#2 Decachlorobiphenyl

R.T.: 8.698 min
Delta R.T.: -0.005 min
Response: 75133367
Conc: 10.99 ng/ml m

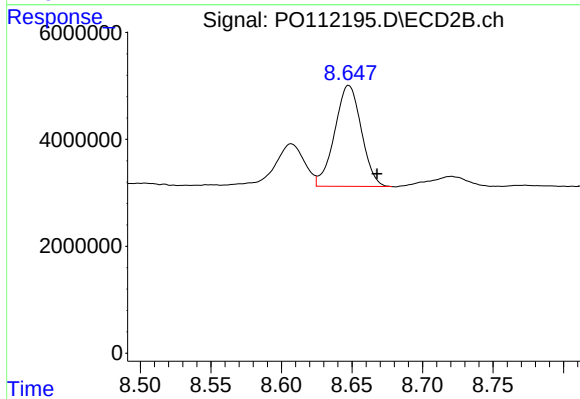

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: -0.021 min
Response: 24784538
Conc: 14.38 ng/ml m